

## TDC7200 Time-to-Digital Converter for Water, Gas, Heat Flow Metering Applications

### 1 Features

- Resolution: 55 ps
- Standard Deviation: 35 ps
- Measurement Range:
  - Mode 1: 12 ns to 500 ns
  - Mode 2: 250 ns to 8 ms
- Low Power Consumption: 0.5  $\mu$ A (2 SPS)
- Supports up to 5 STOP Signals
- Autonomous Multi-Cycle Averaging Mode for Low Power Consumption
- Supply Voltage: 2 V to 3.6 V
- Operating Temperature  $-40^{\circ}\text{C}$  to  $85^{\circ}\text{C}$
- SPI Host Interface for Configuration and Register Access

### 2 Applications

- Flow Meter: Water Meter, Gas Meter, Heat Meter
- Heat Cost Allocators

### 3 Description

The TDC7200 is a Time to Digital Converter (TDC) for ultrasonic sensing measurements such as water flow meter, gas flow meter, and heat flow meter. When paired with the TDC1000 (ultrasonic analog-front-end), the TDC7200 can be a part of a complete TI ultrasonic sensing solution that includes the MSP430, power, wireless, and source code.

The Time to Digital Converter (TDC) performs the function of a stopwatch and measures the elapsed time (time-of-flight or TOF) between a START pulse and up to five STOP pulses. The ability to measure from START to multiple STOPs gives users the flexibility to select which STOP pulse yields the best echo performance.


The device has an internal self-calibrated time base which compensates for drift over time and temperature. Self-calibration enables time-to-digital conversion accuracy in the order of picoseconds. This accuracy makes the TDC7200 ideal for flow meter applications, where zero and low flow measurements require high accuracy.

When placed in the Autonomous Multi-Cycle Averaging Mode, the TDC7200 can be optimized for low system power consumption, making it ideal for battery powered flow meters. In this mode, the host can go to sleep to save power, and it can wake up when interrupted by the TDC upon completion of the measurement sequence.

#### Device Information<sup>(1)</sup>

| PART NUMBER | PACKAGE    | BODY SIZE (NOM)   |
|-------------|------------|-------------------|
| TDC7200     | TSSOP (14) | 5.00 mm x 4.40 mm |

(1) For all available packages, see the orderable addendum at the end of the data sheet.

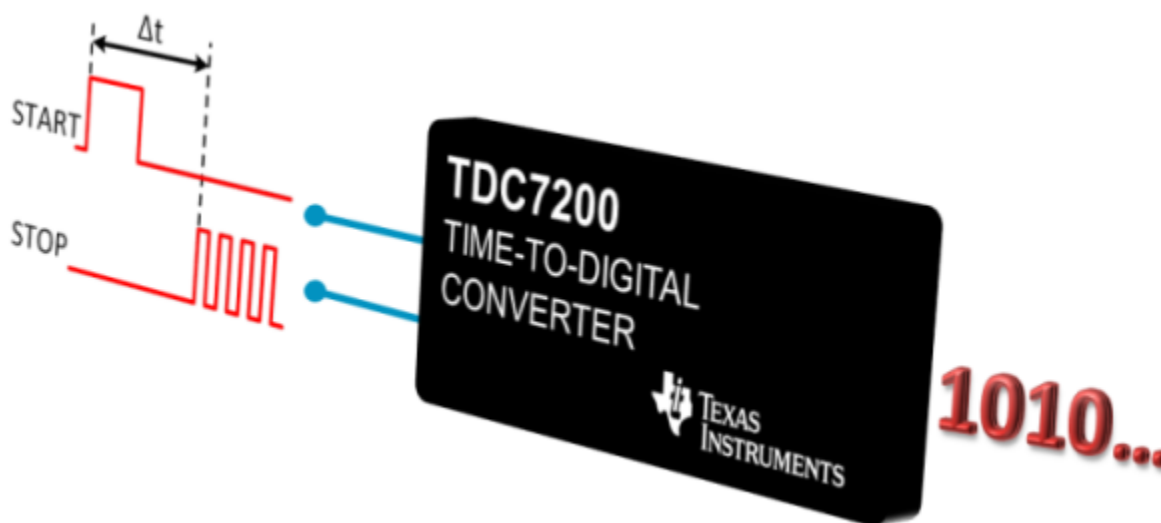

## Table of Contents

|  |           |  |           |
|--|-----------|--|-----------|
| <b>1 Features</b> .....                        | <b>1</b>  | 8.4 Device Functional Modes.....                                 | <b>13</b> |
| <b>2 Applications</b> .....                    | <b>1</b>  | 8.5 Programming.....   | <b>20</b> |
| <b>3 Description</b> .....                     | <b>1</b>  | 8.6 Register Maps .....  | <b>23</b> |
| <b>4 Revision History</b> .....                | <b>2</b>  | <b>9 Application and Implementation</b> .....                    | <b>34</b> |
| <b>5 Companion Device</b> .....                | <b>2</b>  | 9.1 Application Information.....                                 | <b>34</b> |
| <b>6 Pin Configuration and Functions</b> ..... | <b>3</b>  | 9.2 Typical Application .....                                    | <b>34</b> |
| <b>7 Specifications</b> .....                  | <b>4</b>  | 9.3 Post Filtering Recommendations .....                         | <b>38</b> |
| 7.1 Absolute Maximum Ratings .....             | <b>4</b>  | 9.4 CLOCK Recommendations.....                                   | <b>38</b> |
| 7.2 ESD Ratings .....                          | <b>4</b>  | <b>10 Power Supply Recommendations</b> .....                     | <b>40</b> |
| 7.3 Recommended Operating Conditions.....      | <b>4</b>  | <b>11 Layout</b> .....   | <b>40</b> |
| 7.4 Thermal Information .....                  | <b>5</b>  | 11.1 Layout Guidelines .....                                     | <b>40</b> |
| 7.5 Electrical Characteristics.....            | <b>6</b>  | 11.2 Layout Example .....  | <b>41</b> |
| 7.6 Timing Requirements .....                  | <b>6</b>  | <b>12 Device and Documentation Support</b> .....                 | <b>42</b> |
| 7.7 Switching Characteristics .....            | <b>6</b>  | 12.1 Documentation Support .....                                 | <b>42</b> |
| 7.8 Typical Characteristics .....              | <b>8</b>  | 12.2 Trademarks .....  | <b>42</b> |
| <b>8 Detailed Description</b> .....            | <b>11</b> | 12.3 Electrostatic Discharge Caution.....                        | <b>42</b> |
| 8.1 Overview .....                             | <b>11</b> | 12.4 Glossary .....  | <b>42</b> |
| 8.2 Functional Block Diagram .....             | <b>11</b> | <b>13 Mechanical, Packaging, and Orderable Information</b> ..... | <b>42</b> |
| 8.3 Feature Description.....                   | <b>11</b> |  |           |

## 4 Revision History

### Changes from Original (February 2015) to Revision A


**Page**

|                                  |          |
|----------------------------------|----------|
| • Added rest of data sheet. .... | <b>1</b> |
| • Changed ESD Ratings table..... | <b>4</b> |

## 5 Companion Device

| PART NO. | TITLE  |
|----------|--|
| TDC1000  | Ultrasonic Sensing Analog Front End for Level, Concentration, Flow and Proximity Sensing |

## 6 Pin Configuration and Functions

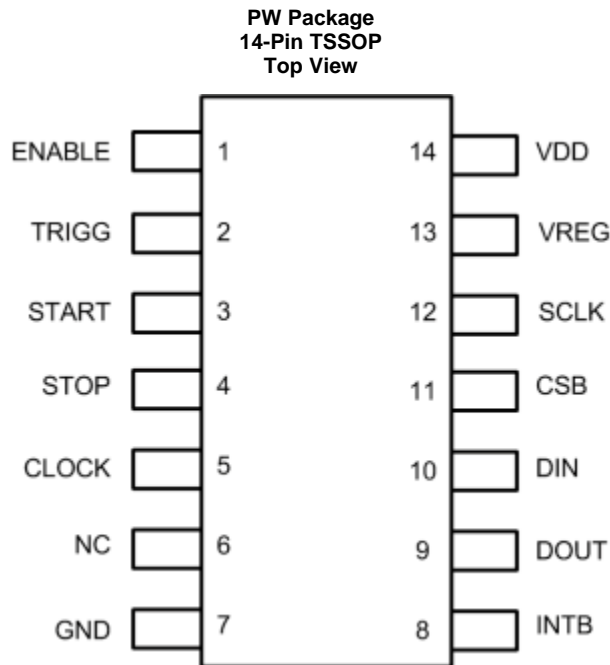

**Pin Functions**

| PIN    |     | I/O    | DESCRIPTION                                     |
|--------|-----|--------|---|
| NAME   | NO. |        |   |
| ENABLE | 1   | Input  | Enable signal to TDC                            |
| TRIGG  | 2   | Output | Trigger output signal                           |
| START  | 3   | Input  | START signal to TDC                             |
| STOP   | 4   | Input  | STOP signal to TDC                              |
| CLOCK  | 5   | Input  | Clock Input to TDC                              |
| N.C.   | 6   | –      | Not Connected                                   |
| GND    | 7   | Ground | Ground  |
| INTB   | 8   | Output | Interrupt to MCU, active low (open drain)       |
| DOUT   | 9   | Output | SPI Data Output                                 |
| DIN    | 10  | Input  | SPI Data Input                                  |
| CSB    | 11  | Input  | SPI Chip Select, active low                     |
| SCLK   | 12  | Input  | SPI clock                                       |
| VREG   | 13  | Output | LDO Output terminal for external decoupling cap |
| VDD    | 14  | Power  | Supply input                                    |

## 7 Specifications

### 7.1 Absolute Maximum Ratings

 $T_A = 25^\circ\text{C}$ ,  $V_{DD} = 3.3\text{V}$ ,  $GND = 0\text{V}$  (unless otherwise noted).<sup>(1)(2)(3)</sup>

|                          |   | MIN  | MAX          | UNIT             |
|--------------------------|---|------|--------------|------------------|
| $V_{DD}$                 | Supply voltage  | -0.3 | 3.9          | V                |
| $V_I$                    | Terminal input voltage  | -0.3 | $V_{DD}+0.3$ | V                |
| $V_{DIFF\_IN}$           | Voltage differential  between any two input terminals           |      | 3.9          | V                |
| $V_{IN\_GND\_V}$<br>$DD$ | Voltage differential  between any input terminal and GND or VDD |      | 3.9          | V                |
| $I_I$                    | Input current at any pin  | -5   | 5            | mA               |
| $T_A$                    | Ambient temperature   | -40  | 125          | $^\circ\text{C}$ |
| $T_{stg}$                | Storage temperature   | -65  | 150          | $^\circ\text{C}$ |

- (1) Stresses beyond those listed under *Absolute Maximum Ratings* may cause permanent damage to the device. These are stress ratings only, which do not imply functional operation of the device at these or any other conditions beyond those indicated under *Recommended Operating Conditions*. Exposure to absolute-maximum-rated conditions for extended periods may affect device reliability.
- (2) The algebraic convention, whereby the most negative value is a minimum and the most positive value is a maximum
- (3) All voltages are with respect to ground, unless otherwise specified.

### 7.2 ESD Ratings

|             |  | VALUE      | UNIT |
|-------------|--|------------|------|
| $V_{(ESD)}$ | Electrostatic discharge  |            | V    |
|             | Human-body model (HBM), per ANSI/ESDA/JEDEC JS-001 <sup>(1)</sup>              | $\pm 1000$ |      |
|             | Charged-device model (CDM), per JEDEC specification JESD22-C101 <sup>(2)</sup> | $\pm 250$  |      |

- (1) JEDEC document JEP155 states that 500-V HBM allows safe manufacturing with a standard ESD control process.
- (2) JEDEC document JEP157 states that 250-V CDM allows safe manufacturing with a standard ESD control process.

### 7.3 Recommended Operating Conditions

 $T_A = 25^\circ\text{C}$ ,  $V_{DD} = 3.3\text{V}$ ,  $GND = 0\text{V}$  (unless otherwise noted).

|  |   | MIN                  | NOM      | MAX                           | UNIT |
|--|---|----------------------|----------|-------------------------------|------|
| $V_{DD}$   | Supply voltage                                | 2                    |          | 3.6                           | V    |
| $V_I$  | Terminal voltage                              | 0                    |          | $V_{DD}$                      | V    |
| $V_{IH}$   | Voltage input high                            | $0.7 \times V_{DD}$  |          | 3.6                           | V    |
| $V_{IL}$   | Voltage input low                             | 0                    |          | $0.3 \times V_{DD}$           | V    |
| $F_{CALIB\_CLK}$   | Frequency (Reference/Calibration Clock)       | 1 <sup>(1)</sup>     | 8        | 16                            | MHz  |
| $DUTY_{CLOCK}$   | Input clock duty cycle                        |                      | 50%      |                               |      |
| <b>TIMING REQUIREMENTS: Measurement Mode 1<sup>(1)</sup></b> |   |                      |          |                               |      |
| $T1_{STARTSTOP\_Min}$  | Minimum Time between Start and Stop Signal    | 12                   |          |                               | ns   |
| $T1_{STOPSTOP\_Min}$   | Minimum Time between 2 Stop Signals           | 67                   |          |                               | ns   |
| $T1_{STARTSTOP\_Max}$  | Maximum time bet. Start and Stop Signal       |                      |          | 500                           | ns   |
| $T1_{STOPSTOP\_Max}$   | Maximum time bet. Start and last Stop Signal  |                      |          | 500                           | ns   |
| <b>TIMING REQUIREMENTS: Measurement 2<sup>(1)</sup></b>      |   |                      |          |                               |      |
| $T2_{STARTSTOP\_Min}$  | Minimum Time between Start and Stop Signal    | $2 \times t_{CLOCK}$ |          |                               | s    |
| $T2_{STOPSTOP\_Min}$   | Minimum Time between 2 Stop Signals           | $2 \times t_{CLOCK}$ |          |                               | s    |
| $T2_{STARTSTOP\_Max}$  | Maximum time bet. Start and Stop Signal       |                      |          | $(2^{16}-2) \times t_{CLOCK}$ | s    |
| $T2_{STOPSTOP\_Max}$   | Maximum. time bet. Start and last Stop Signal |                      |          | $(2^{16}-2) \times t_{CLOCK}$ | s    |
| <b>TIMING REQUIREMENTS: ENABLE INPUT</b>                     |   |                      |          |                               |      |
| $T_{REN}$  | Rise Time for Enable Signal (20%-80%)         |                      | 1 to 100 |                               | ns   |
| $T_{FEN}$  | Fall Time for Enable Signal (20%-80%)         |                      | 1 to 100 |                               | ns   |

- (1) Specified by design.

## Recommended Operating Conditions (continued)

$T_A = 25^\circ\text{C}$  ,  $V_{DD} = 3.3\text{V}$ ,  $GND = 0\text{V}$  (unless otherwise noted).

|  |   | MIN | NOM | MAX | UNIT             |
|--|---|-----|-----|-----|------------------|
| <b>TIMING REQUIREMENTS: START, STOP, CLOCK</b> |   |     |     |     |                  |
| $T_{RST}$ , $T_{FST}$                          | Maximum rise, fall time for START, STOP signals (20%-80%) |     | 1   |     | ns               |
| $T_{RXCLK}$ , $T_{FXCLK}$                      | Maximum rise, fall time for external CLOCK (20%-80%)      |     | 1   |     | ns               |
| <b>TIMING REQUIREMENTS: TRIGG</b>              |   |     |     |     |                  |
| $T_{TRIGSTART}$                                | Time from TRIG to START                                   |     | 5   |     | ns               |
| <b>TEMPERATURE</b>                             |   |     |     |     |                  |
| $T_A$  | Ambient temperature                                       | -40 |     | 85  | $^\circ\text{C}$ |
| $T_J$  | Junction temperature                                      | -40 |     | 85  | $^\circ\text{C}$ |

## 7.4 Thermal Information

| THERMAL METRIC <sup>(1)</sup> |  | TDC7200<br>PW [TSSOP]<br>14 PINS | UNIT                      |
|-------------------------------|--|----------------------------------|---------------------------|
| $R_{\theta JA}$               | Junction-to-ambient thermal resistance       | 134.9                            | $^\circ\text{C}/\text{W}$ |
| $R_{\theta JC(top)}$          | Junction-to-case (top) thermal resistance    | 63                               |                           |
| $R_{\theta JB}$               | Junction-to-board thermal resistance         | 76.8                             |                           |
| $\psi_{JT}$                   | Junction-to-top characterization parameter   | 12.4                             |                           |
| $\psi_{JB}$                   | Junction-to-board characterization parameter | 76.2                             |                           |
| $\theta_{JA}$                 | Package thermal impedance                    | 113                              |                           |

(1) For more information about traditional and new thermal metrics, see the *IC Package Thermal Metrics* application report, [SPRA953](#).

## 7.5 Electrical Characteristics

 $T_A = 25^\circ\text{C}$ ,  $V_{DD} = 3.3\text{ V}$ ,  $GND = 0\text{ V}$  (unless otherwise noted).

| PARAMETER  |                                  | TEST CONDITIONS  | MIN  | TYP  | MAX  | UNIT          |
|--|----------------------------------|--|------|------|------|---------------|
| <b>TDC CHARACTERISTICS</b>   |                                  |  |      |      |      |               |
| LSB  | Resolution                       | Single shot measurement                                |      | 55   |      | ps            |
| $T_{ACC-2}$  | Accuracy (Mode 2) <sup>(1)</sup> | CLOCK = 8 MHz  |      | 28   |      | ps            |
| $T_{STD-2}$  | Standard Deviation (Mode 2)      | Measured time = 100 $\mu\text{s}$                      |      | 50   |      | ps            |
|  |                                  | Measured time = 1 $\mu\text{s}$                        |      | 35   |      | ps            |
| <b>OUTPUT CHARACTERISTICS: TRIGG, INTB, DOUT</b>   |                                  |  |      |      |      |               |
| $V_{OH}$   | Output voltage high              | $I_{source} = -2\text{ mA}$                            | 2.31 | 2.95 |      | V             |
| $V_{OL}$   | Output voltage low               | $I_{sink} = 2\text{ mA}$                               |      | 0.35 | 0.99 | V             |
| <b>INPUT CHARACTERISTICS: ENABLE, START, STOP, CLOCK, DIN, CSB,SCLK</b>                                  |                                  |  |      |      |      |               |
| $C_{in}$   | Input capacitance <sup>(2)</sup> |  |      | 3    |      | pF            |
| <b>POWER CONSUMPTION (see <a href="#">Measurement Mode 1</a> and <a href="#">Measurement Mode 2</a>)</b> |                                  |  |      |      |      |               |
| $I_{sh}$   | Shutdown current                 | EN = LOW   |      | 0.3  | 2    | $\mu\text{A}$ |
| $I_{QA}$   | Quiescent Current A              | EN = HIGH; TDC running                                 |      | 1.35 |      | mA            |
| $I_{QB}$   | Quiescent Current B              | EN = HIGH; TDC OFF, Clock Counter running              |      | 71   |      | $\mu\text{A}$ |
| $I_{QC}$   | Quiescent Current C              | EN = HIGH; measurement stopped, SPI communication only |      | 87   |      | $\mu\text{A}$ |
| $I_{QD}$   | Quiescent Current D              | TDC OFF, counter stopped, no communication             |      | 50   |      | $\mu\text{A}$ |

(1) Accuracy is defined as the systematic error in the output signal; the error of the device excluding noise.

(2) Specified by design.

## 7.6 Timing Requirements

|   |  | MIN | NOM | MAX | UNIT |
|---|--|-----|-----|-----|------|
| <b>TIMING REQUIREMENTS: START, STOP INPUTS, CLOCK</b>   |  |     |     |     |      |
| $PW_{START}$  | Pulse width for Start Signal             | 10  |     |     | ns   |
| $PW_{STOP}$   | Pulse width for Stop Signal              | 10  |     |     | ns   |
| <b>SERIAL INTERFACE TIMING CHARACTERISTICS (<math>V_{DD} = 3.3\text{ V}</math>, <math>f_{SCLK} = 20\text{ MHz}</math>) (See <a href="#">Figure 1</a>)</b> |  |     |     |     |      |
| $f_{SCLK}$  | SCLK Frequency                           |     |     | 20  | MHz  |
| $t_1$   | SCLK period                              | 50  |     |     | ns   |
| $t_2$   | SCLK High Time                           | 16  |     |     | ns   |
| $t_3$   | SCLK Low Time                            | 16  |     |     | ns   |
| $t_4$   | DIN setup time                           | 4   |     |     | ns   |
| $t_5$   | DIN hold time                            | 4   |     |     | ns   |
| $t_6$   | CSB fall to SCLK rise                    | 6   |     |     | ns   |
| $t_7$   | Last SCLK rising edge to CSB rising edge | 6   |     |     | ns   |
| $t_8$   | Minimum pause time (CSB high)            | 40  |     |     | ns   |
| $t_9$   | Clk fall to DOUT bus transition          |     |     | 12  | ns   |

## 7.7 Switching Characteristics

 $T_A = 25^\circ\text{C}$ ,  $V_{DD} = 3.3\text{ V}$ ,  $GND = 0\text{ V}$  (unless otherwise noted).

| PARAMETER            |                                  | TEST CONDITIONS                  | MIN | TYP | MAX | UNIT          |
|----------------------|----------------------------------|----------------------------------|-----|-----|-----|---------------|
| <b>WAKE UP TIME</b>  |                                  |                                  |     |     |     |               |
| $T_{WAKEUP\_PERIOD}$ | Time to be ready for Measurement | LSB within 0.3% of settled value |     | 300 |     | $\mu\text{s}$ |

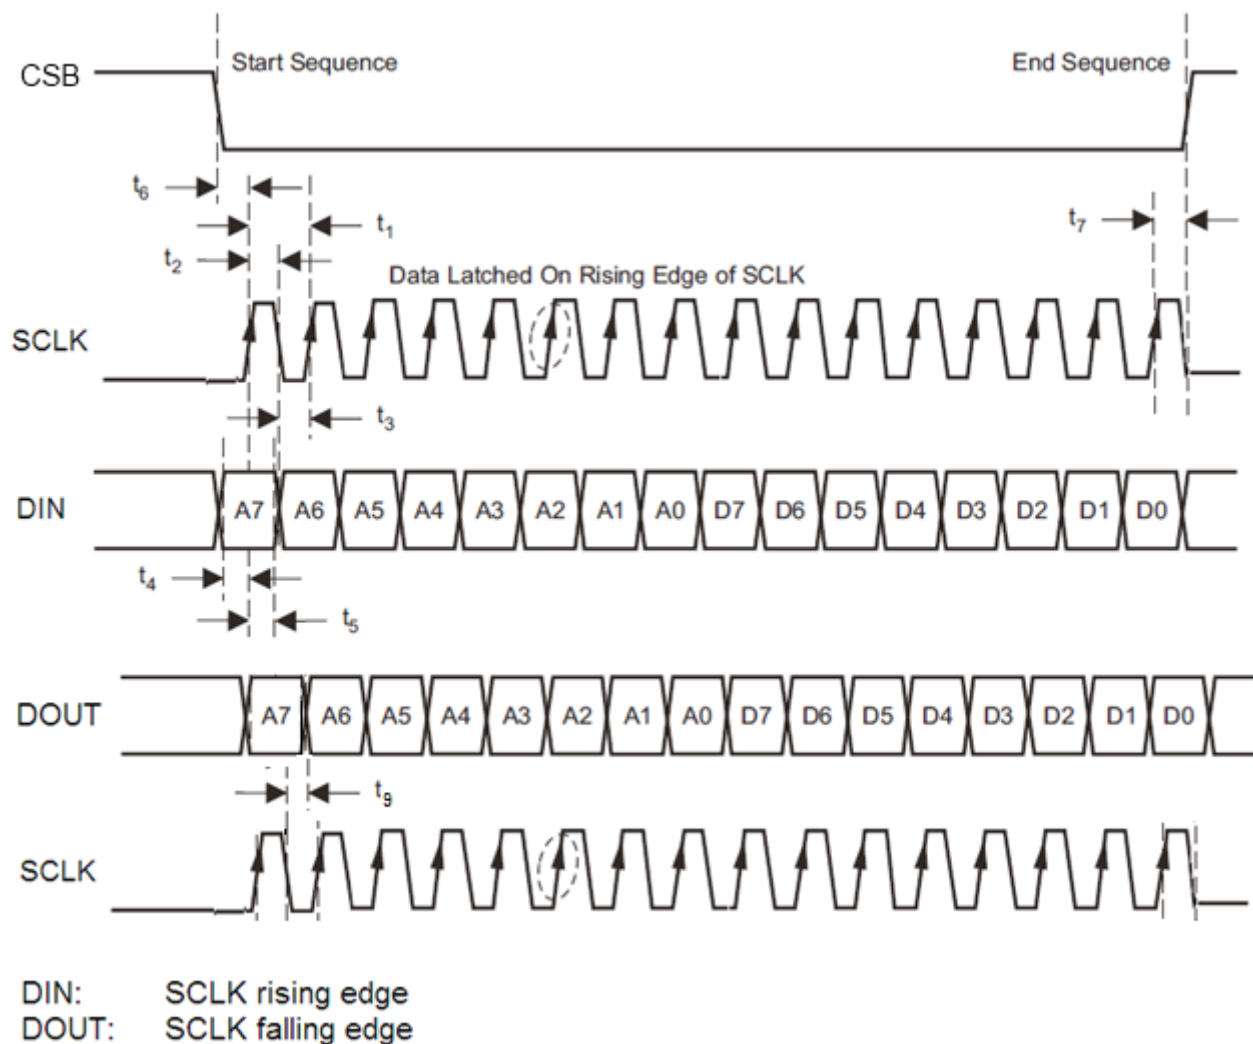


Figure 1. SPI Register Write: 8 bit Register Example

### 7.8 Typical Characteristics

T<sub>A</sub> = 25°C , V<sub>DD</sub> = 3.3 V, GND = 0 V, CLOCK = 8 MHz, CALIBRATION2\_PERIODS = 10, AVG\_CYCLES = 1 Measurement, NUM\_STOP = Single STOP, Measurement Mode 2 (unless otherwise noted).

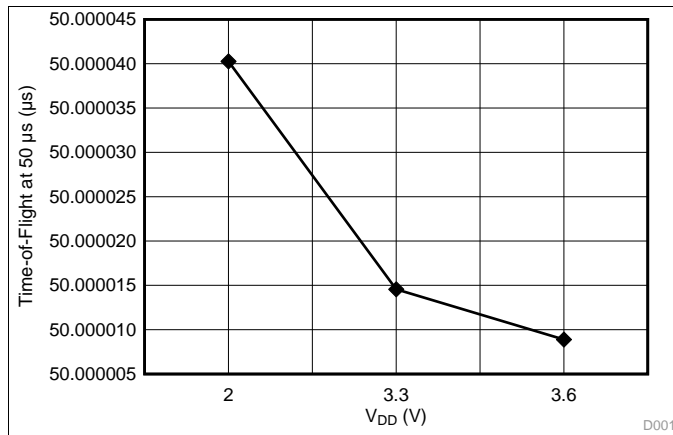


Figure 2. Time-of-Flight (TOF) vs. VDD (Measurement Mode 2)

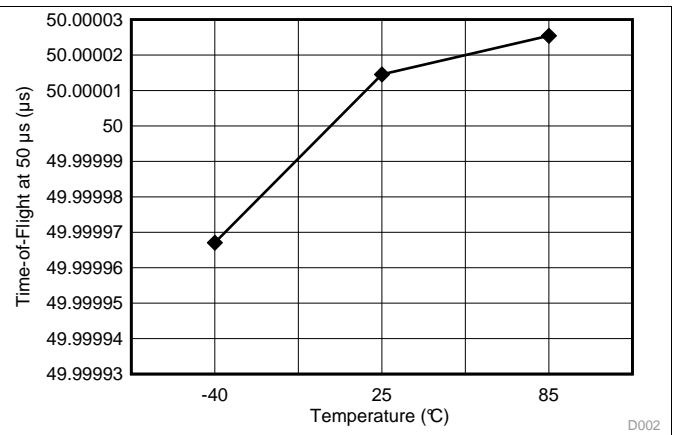


Figure 3. TOF vs. Temperature (Measurement Mode 2)

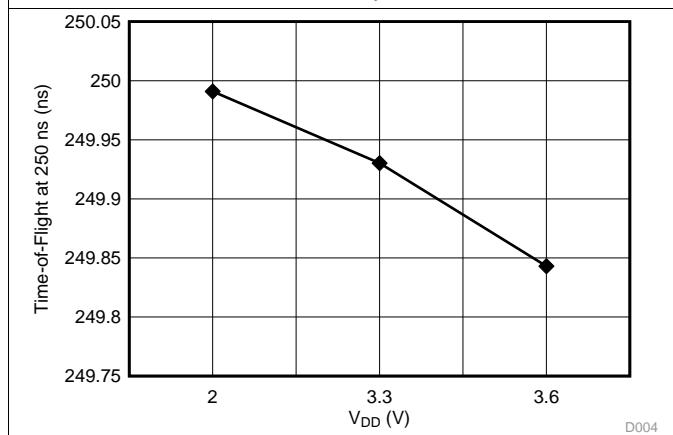


Figure 4. TOF vs. VDD (Measurement Mode 1)

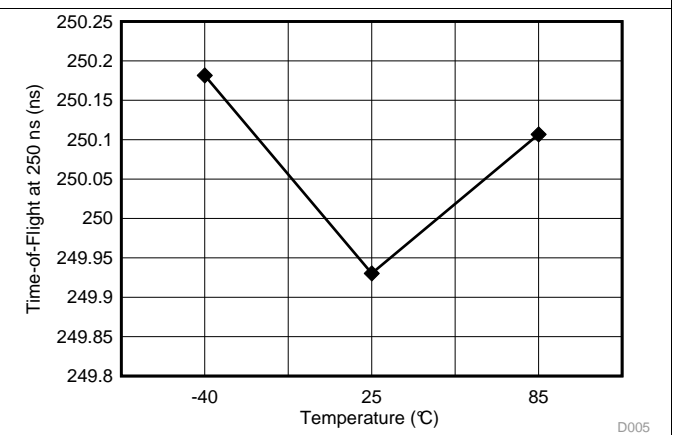


Figure 5. TOF vs. Temperature (Measurement Mode 1)

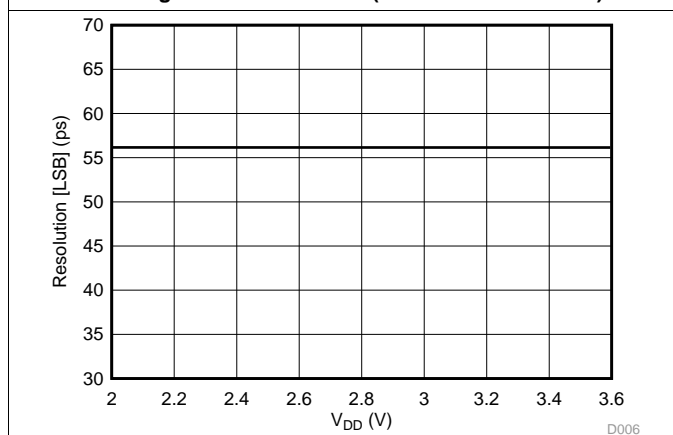


Figure 6. Resolution (LSB) vs. VDD


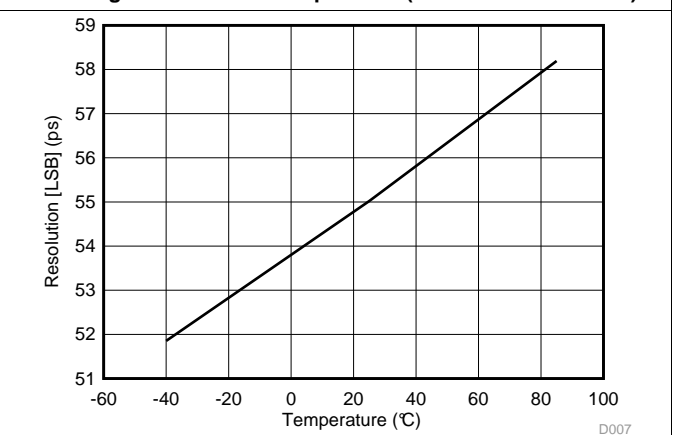


Figure 7. Resolution (LSB) vs. Temperature


Typical Characteristics (continued)

T<sub>A</sub> = 25°C, V<sub>DD</sub> = 3.3 V, GND = 0 V, CLOCK = 8 MHz, CALIBRATION2\_PERIODS = 10, AVG\_CYCLES = 1 Measurement, NUM\_STOP = Single STOP, Measurement Mode 2 (unless otherwise noted).

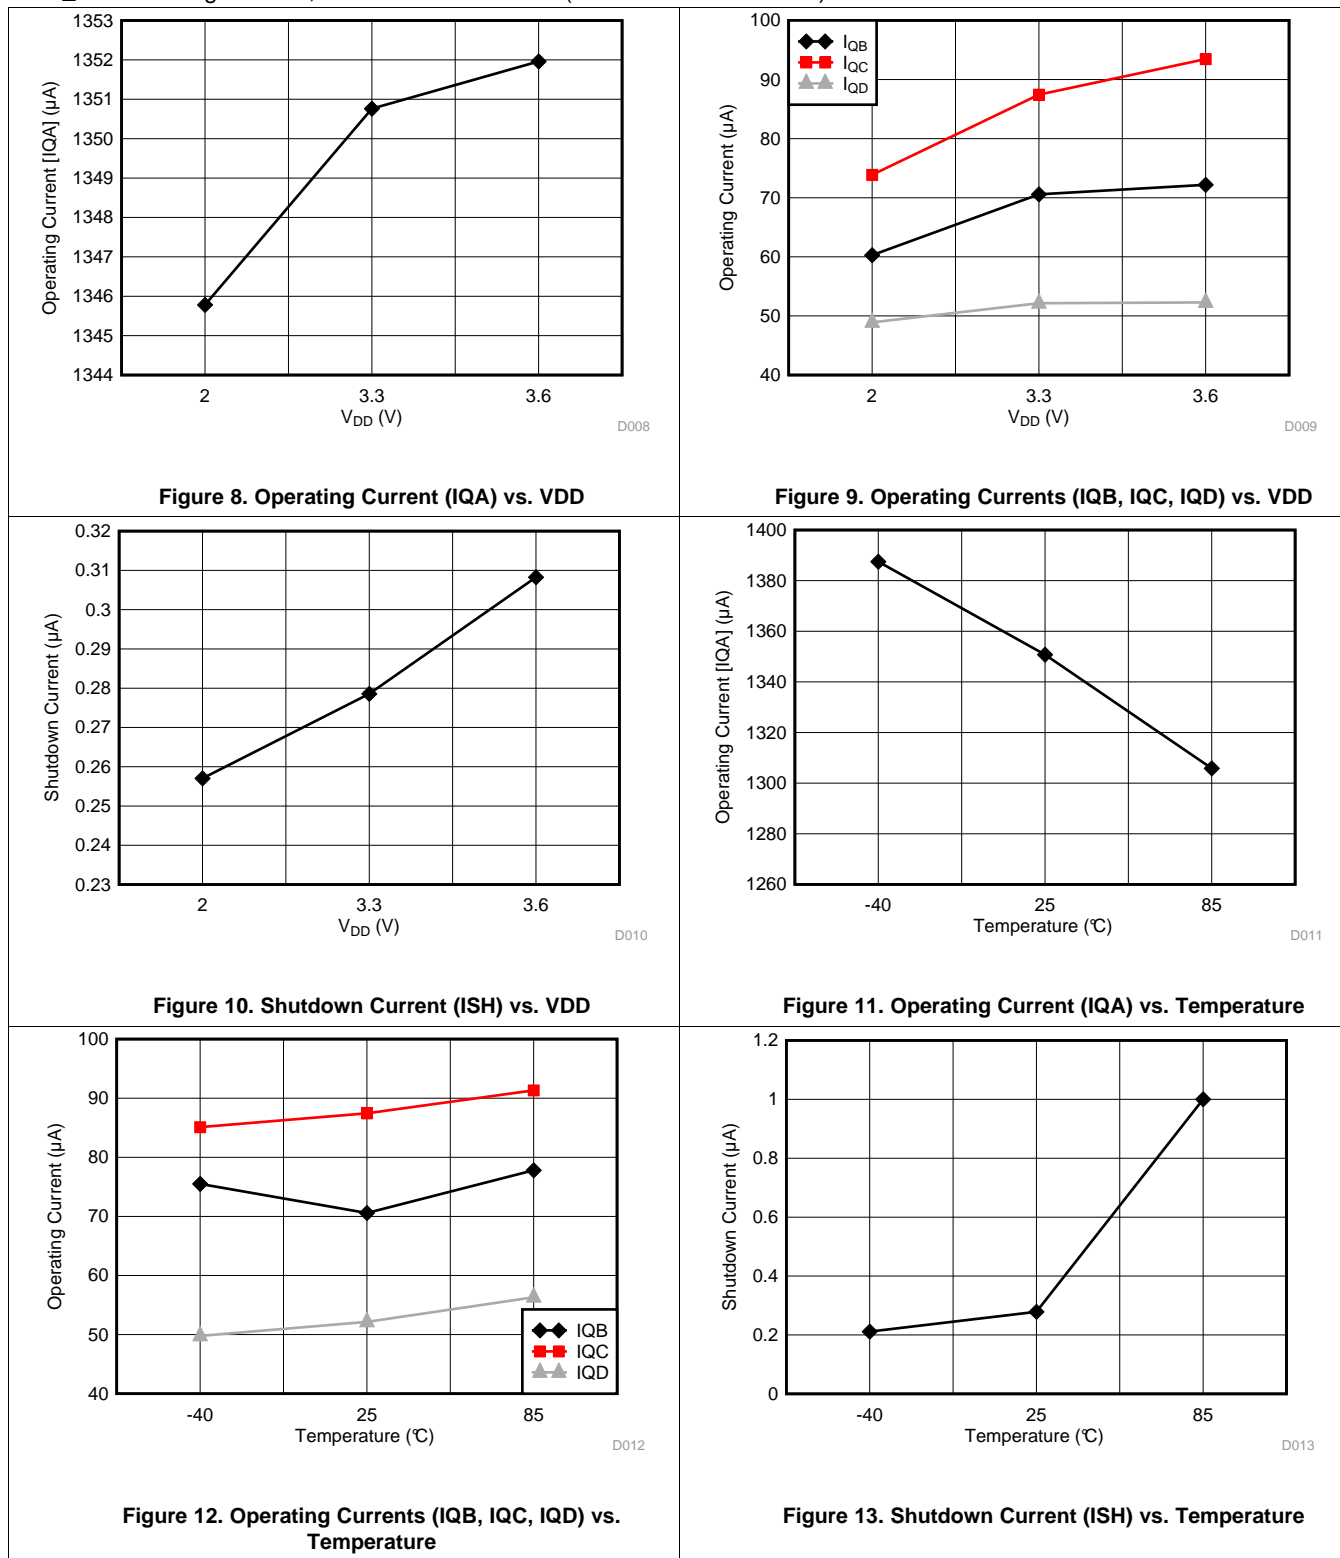

**Typical Characteristics (continued)**

$T_A = 25^\circ\text{C}$  ,  $V_{DD} = 3.3\text{ V}$  ,  $GND = 0\text{ V}$  ,  $CLOCK = 8\text{ MHz}$  ,  $CALIBRATION2\_PERIODS = 10$  ,  $AVG\_CYCLES = 1$  Measurement,  
 $NUM\_STOP = \text{Single STOP}$  , Measurement Mode 2 (unless otherwise noted).

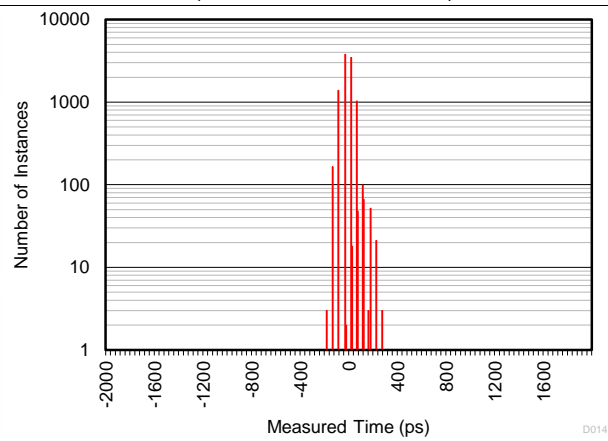


**Figure 14. Standard Time-of-Flight Histogram (Normalized)**

## 8 Detailed Description

### 8.1 Overview

The TDC7200 is a stopwatch IC used to measure time between a single event (edge on START pin) and multiple subsequent events (edge on STOP pin). An event from a START pulse to a STOP pulse is also known as time-of-flight, or TOF for short. The device has an internal time base that is used to measure time with accuracy in the order of picoseconds. This accuracy makes the TDC7200 ideal for application such as flow meter, where zero and low flow measurements require high accuracy in the picoseconds range.

### 8.2 Functional Block Diagram

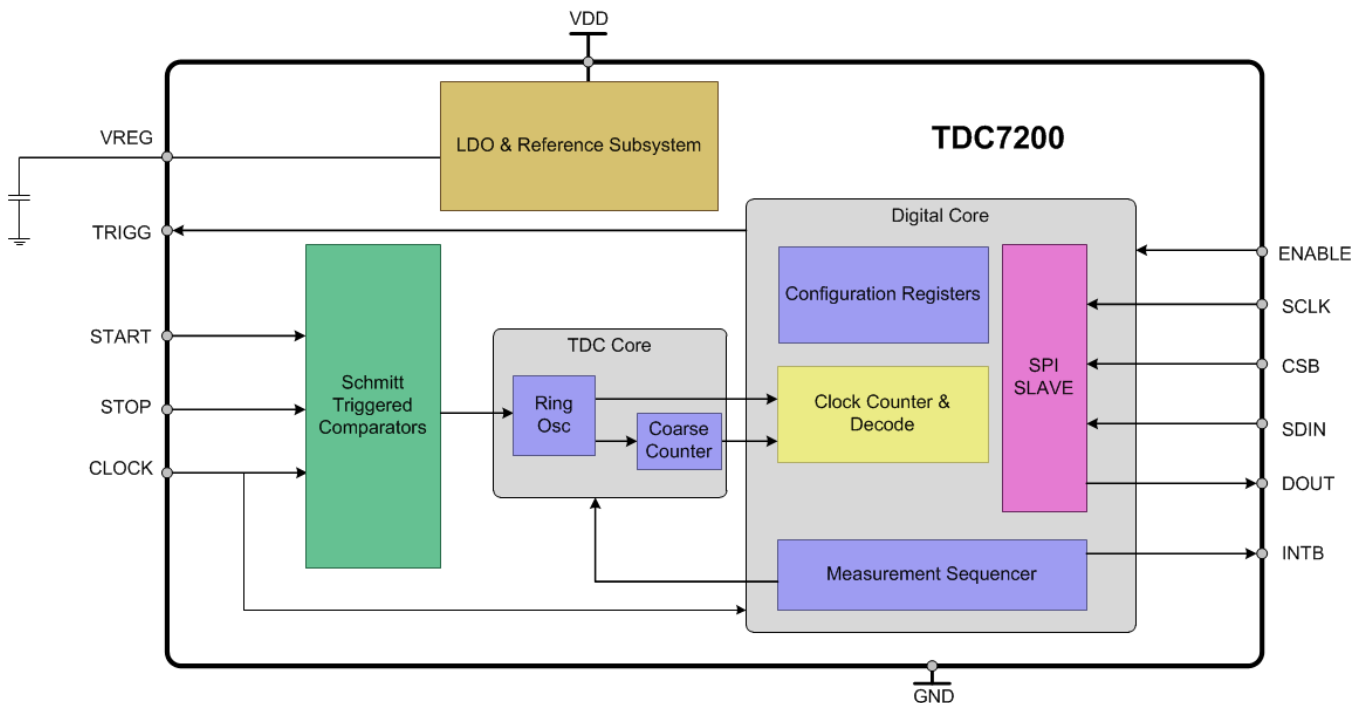

### 8.3 Feature Description

#### 8.3.1 LDO

The LDO (low-dropout) is an internal supply voltage regulator for the TDC7200. No external circuitry needs to be connected to the output of this regulator other than the mandatory external decoupling capacitor.

Recommendations for the decoupling capacitor parameters:


- Type: ceramic
- Capacitance: 0.4  $\mu\text{F}$ –2.7  $\mu\text{F}$  (1  $\mu\text{F}$  typical). If using a capacitor value outside the recommended range, the part may malfunction and can be damaged.
- ESR: 100 m $\Omega$  (max)

## Feature Description (continued)

### 8.3.2 CLOCK

TDC7200 needs an external reference clock connected to the CLOCK pin. The external CLOCK is used to calibrate the internal time base accurately and therefore, the measurement accuracy is heavily dependent on the external CLOCK accuracy. This reference clock is also used by all digital circuits inside the device; thus, CLOCK has to be available and stable at all times when the device is enabled (ENABLE = HIGH).

Figure 15 shows the typical effect of the external CLOCK frequency on the measurement uncertainty. With a reference clock of 1MHz, the standard deviation of a set of measurement results is approximately 243ps. As the reference clock frequency is increased, the standard deviation (or measurement uncertainty) reduces. Therefore, using a reference clock of 16MHz is recommended for optimal performance.

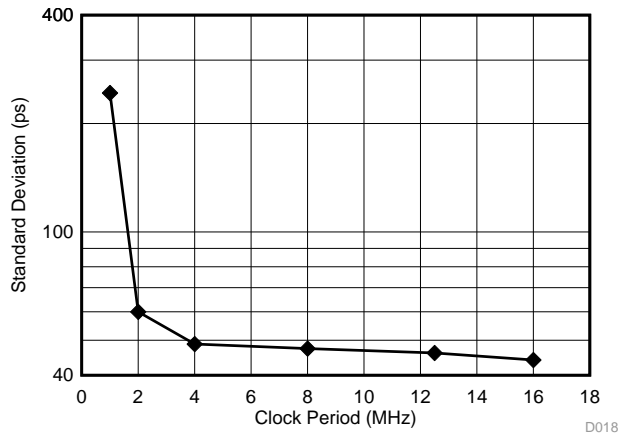

**Figure 15. Standard Deviation vs. CLOCK**

### 8.3.3 Counters

#### 8.3.3.1 Coarse and Clock Counters Description

Time measurements by the TDC7200 rely on two counters: the Coarse Counter and the Clock Counter. The Coarse Counter counts the number of times the ring oscillator (the TDC7200's core time measurement mechanism) wraps, which is used to generate the results in the [TIME1](#) to [TIME6](#) registers.

The Clock Counter counts the number of integer clock cycles between START and STOP events and is used in [Measurement Mode 2](#) only. The results for the Clock Counter are displayed in the [CLOCK\\_COUNT1](#) to [CLOCK\\_COUNT5](#) registers.

#### 8.3.3.2 Coarse and Clock Counters Overflow

Once the coarse counter value has reached the corresponding value of the Coarse Counter Overflow registers, then its interrupt bit will be set to 1. In other words, if  $(\text{TIME}_n / 63) \geq \text{COARSE\_CNTR\_OVF}$ , then  $\text{COARSE\_CNTR\_OVF\_INT} = 1$  (this interrupt bit is located in the [INT\\_STATUS](#) register).  $\text{COARSE\_CNTR\_OVF} = (\text{COARSE\_CNTR\_OVF\_H} \times 2^8 + \text{COARSE\_CNTR\_OVF\_L})$ , and  $\text{TIME}_n$  refers to the [TIME1](#) to [TIME6](#) registers.

Similarly, once the clock counter value has reached the corresponding value of the Clock Counter Overflow registers, then its interrupt bit will be set to 1. In other words, if  $\text{CLOCK\_COUNT}_n > \text{CLOCK\_CNTR\_OVF}$ , then  $\text{CLOCK\_CNTR\_OVF\_INT} = 1$  (this interrupt bit is located in the [INT\\_STATUS](#) register).  $\text{CLOCK\_CNTR\_OVF} = (\text{CLOCK\_CNTR\_OVF\_H} \times 2^8 + \text{CLOCK\_CNTR\_OVF\_L})$ , and  $\text{CLOCK\_COUNT}_n$  refers to the [CLOCK\\_COUNT1](#) to [CLOCK\\_COUNT5](#) registers.

As soon as there is an overflow detected, the running measurement will be terminated immediately.

## Feature Description (continued)

### 8.3.3.3 Clock Counter STOP Mask

The value in the Clock Counter STOP Mask registers define the end of the mask window. The Clock Counter STOP Mask value will be referred to as  $CLOCK\_CNTR\_STOP\_MASK = (CLOCK\_CNTR\_STOP\_MASK\_H \times 2^8 + CLOCK\_CNTR\_STOP\_MASK\_L)$ .

The Clock Counter is started by the first rising edge of the external CLOCK after the START signal (see [Figure 18](#)). All STOP signals occurring before the value set by the  $CLOCK\_CNTR\_STOP\_MASK$  registers will be ignored. This feature can be used to help suppress wrong or unwanted STOP trigger signals.

For example, assume the following values:

- The first time-of-flight (TOF1), which is defined as the time measurement from the START to the 1<sup>st</sup> STOP = 19  $\mu$ s.
- The second time-of-flight (TOF2), which is defined as the time measurement from the START to the 2<sup>nd</sup> STOP = 119  $\mu$ s.
- CLOCK = 8 MHz

In this example, the TDC7200 will provide a [CLOCK\\_COUNT1](#) of approximately 152 ( $19 \mu\text{s} / t_{\text{CLOCK}}$ ), and [CLOCK\\_COUNT2](#) of approximately 952 ( $119 \mu\text{s} / t_{\text{CLOCK}}$ ). If the user sets  $CLOCK\_CNTR\_STOP\_MASK$  anywhere between 152 and 952, then the 1<sup>st</sup> STOP will be ignored and 2<sup>nd</sup> STOP will be measured.

The Clock Counter Overflow value ( $CLOCK\_CNTR\_OVF\_H \times 2^8 + CLOCK\_CNTR\_OVF\_L$ ) should always be higher than the Clock Counter STOP Mask value ( $\times 2^8 + CLOCK\_CNTR\_STOP\_MASK\_L$ ). Otherwise, the Clock Counter Overflow Interrupt will be set before the STOP mask time expires, and the measurement will be halted.

### 8.3.3.4 ENABLE

The ENABLE pin is used as a reset to all digital circuits in the TDC7200. Therefore, it is essential that the ENABLE pin sees a positive edge after the device has powered up. It is also important to ensure that there are no transients (glitches, etc.) on the ENABLE pin; such glitches could cause the device to RESET.

## 8.4 Device Functional Modes

### 8.4.1 Calibration

The time measurements performed by the TDC7200 are based on an internal time base which is represented as the LSB value of the [TIME1](#) to [TIME6](#) results registers. The typical LSB value can be seen in [Electrical Characteristics](#). However, the actual value of the LSB can vary depending on environmental variables (temperature, systematic noise, etc.). This variation can introduce significant error into the measurement result. There is also an offset error in the measurement due to certain internal delays in the device.

In order to compensate for these errors and to calculate the actual LSB value, calibration needs to be performed. The TDC7200 calibration consists of two measurement cycles of the external CLOCK. The first is a measurement of a single clock cycle period of the external clock; the second measurement is for the number of external CLOCK periods set by the CALIBRATION2\_PERDIOS in the [CONFIG2](#) register. The results from the calibration measurements are stored in the [CALIBRATION1](#) and [CALIBRATION2](#) registers.

The two-point calibration is used to determine the actual LSB in real time in order to convert the [TIME1](#) to [TIME6](#) results from number of delays to a real time-of-flight (TOF) number. As discussed in the next sections, the calibrations will be used for calculating time-of-flight (TOF) in measurement modes 1 and 2.

## Device Functional Modes (continued)

### 8.4.2 Measurement Modes

#### 8.4.2.1 Measurement Mode 1

In measurement mode 1 as shown in Figure 16, the TDC7200 performs the entire counting from START to the last STOP using its internal ring oscillator plus coarse counter. This method is recommended for measuring shorter time durations of **< 500 ns**. Using measurement mode 1 for measuring time > 500ns decreases accuracy of the measurement (as shown in Figure 17), **and is not recommended**.

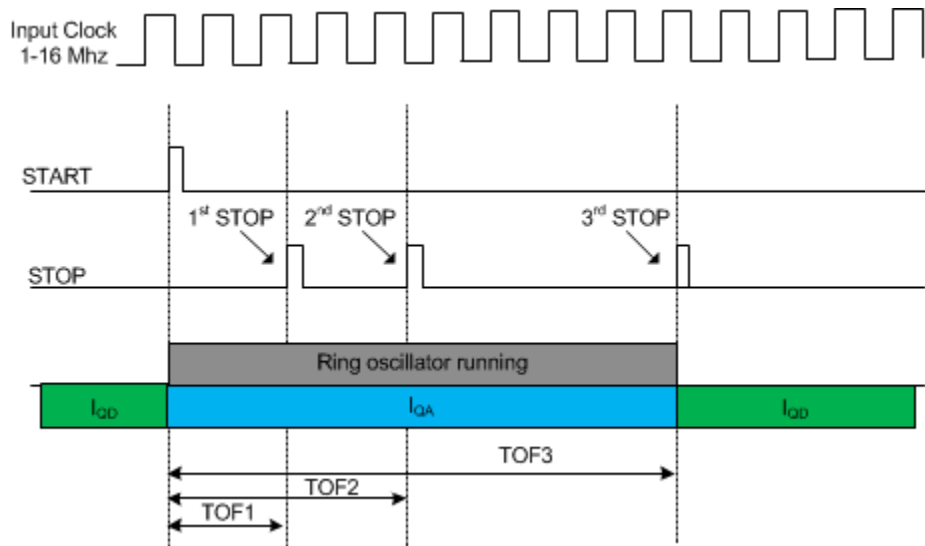


Figure 16. Measurement Mode 1

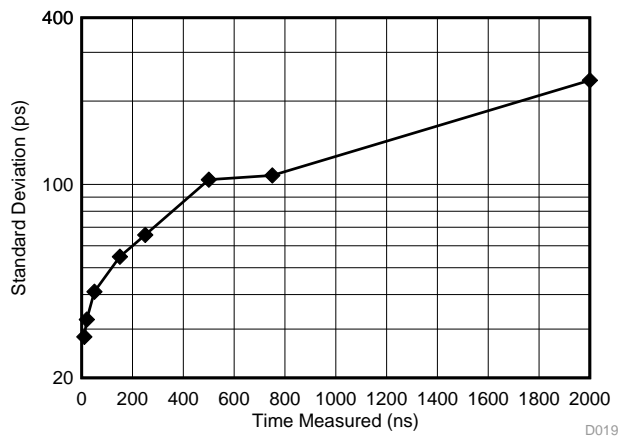


Figure 17. Measurement Mode 1 Standard Deviation vs. Measured Time-of-Flight

## Device Functional Modes (continued)

### 8.4.2.1.1 Calculating Time-of-Flight (Measurement Mode 1)

For measurement mode 1, the time-of-flight (TOF) between the START to the n<sup>th</sup> STOP can be calculated using Equation 1:

$$\begin{aligned} \text{TOF}_n &= (\text{TIME}_n)(\text{normLSB}) \\ \text{normLSB} &= \frac{(\text{CLOCKperiod})}{(\text{calCount})} \\ \text{calCount} &= \frac{\text{CALIBRATION2} - \text{CALIBRATION1}}{(\text{CALIBRATION2\_PERIODS}) - 1} \end{aligned}$$

where

- $\text{TOF}_n$  [sec] = time-of-flight measurement from the START to the n<sup>th</sup> STOP
- $\text{TIME}_n$  = n<sup>th</sup> TIME measurement given by the [TIME1](#) to [TIME6](#) registers
- normLSB [sec] = normalized LSB value from calibration
- CLOCKperiod [sec] = external CLOCK period
- [CALIBRATION1](#) [count] = TDC count for first calibration cycle
- [CALIBRATION2](#) [count] = TDC count for second calibration cycle
- CALIBRATION2\_PERIODS = setting for the second calibration cycle; located in register [CONFIG2](#) (1)

For example, assume the time-of-flight between the START to the 1<sup>st</sup> STOP is desired, and the following readouts were obtained:

- CALIBRATION2 = 21121 (decimal)
- CALIBRATION1 = 2110 (decimal)
- CALIBRATION2\_PERIODS = 10
- CLOCK = 8MHz
- TIME1 = 4175 (decimal)


Therefore, the calculation for time-of-flight is:

- $\text{calCount} = (21121 - 2110) / (10 - 1) = 2112.33$
- $\text{normLSB} = (1/8\text{MHz}) / (2112.33) = 5.917 \times 10^{-11}$
- $\text{TOF1} = (4175)(5.917 \times 10^{-11}) = 247.061 \text{ ns}$

### 8.4.2.2 Measurement Mode 2

In measurement mode 2, the internal ring oscillator of the TDC7200 is used only to count fractional parts of the total measured time. As shown in [Figure 18](#), the internal ring oscillator starts counting from when it receives the START signal until the first rising edge of the CLOCK. Then, the internal ring oscillator switches off, and the Clock counter starts counting the clock cycles of the external CLOCK input until a STOP pulse is received. The internal ring oscillator again starts counting from the STOP signal until the next rising edge of the CLOCK.

**Device Functional Modes (continued)**

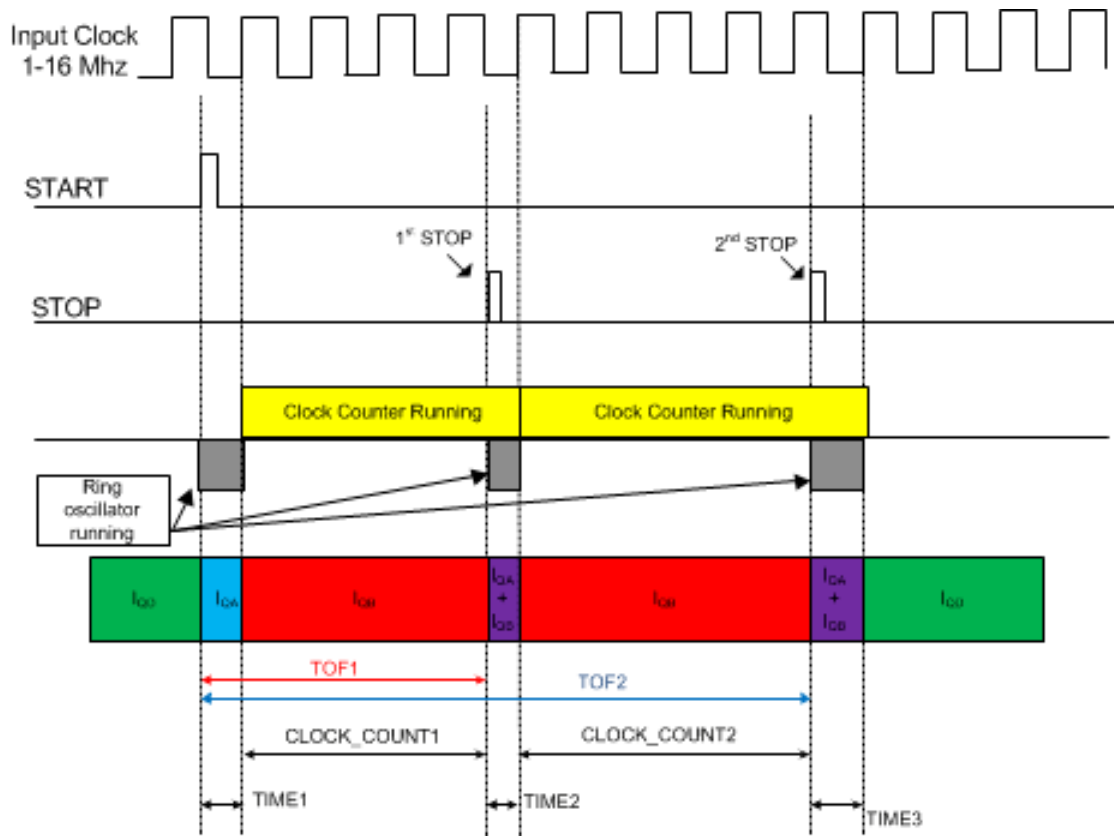

**Figure 18. Measurement Mode 2**

## Device Functional Modes (continued)

### 8.4.2.2.1 Calculating Time-of-Flight (TOF) (Measurement Mode 2)

The time-of-flight (TOF) between the START to the  $n^{\text{th}}$  STOP can be calculated using [Equation 2](#):

$$\text{TOF}_n = \text{normLSB}(\text{TIME1} - \text{TIME}_{n+1}) + (\text{CLOCK\_COUNT}_n)(\text{CLOCKperiod})$$

$$\text{normLSB} = \frac{(\text{CLOCKperiod})}{(\text{calCount})}$$

$$\text{calCount} = \frac{\text{CALIBRATION2} - \text{CALIBRATION1}}{(\text{CALIBRATION2\_PERIODS}) - 1}$$

$$\text{offset} = \text{CLOCKperiod} - (\text{CALIBRATION1})(\text{normLSB})$$

where

- $\text{TOF}_n$  [sec] = time-of-flight measurement from the START to the  $n^{\text{th}}$  STOP
- [TIME1](#) = time 1 measurement given by the TDC7200 register address 0x10
- $\text{TIME}_{(n+1)}$  = (n+1) time measurement, where n = 1 to 5 ([TIME2](#) to [TIME6](#) registers)
- normLSB [sec] = normalized LSB value from calibration
- $\text{CLOCK\_COUNT}_n$  = nth clock count, where n = 1 to 5 ([CLOCK\\_COUNT1](#) to [CLOCK\\_COUNT5](#))
- CLOCKperiod [sec] = external CLOCK period
- [CALIBRATION1](#) [count] = TDC count for first calibration cycle
- [CALIBRATION2](#) [count] = TDC count for second calibration cycle
- CALIBRATION2\_PERIODS = setting for the second calibration; located in register [CONFIG2](#) (2)

For example, assume the time-of-flight between the START to the 1<sup>st</sup> STOP is desired, and the following readouts were obtained:

- CALIBRATION2 = 23133 (decimal)
- CALIBRATION1 = 2315 (decimal)
- CALIBRATION2\_PERIODS = 10
- CLOCK = 8MHz
- TIME1 = 2147 (decimal)
- TIME2 = 201 (decimal)
- CLOCK\_COUNT1 = 3818 (decimal)

Therefore, the calculation for time-of-flight is:

$$\text{calCount} = \frac{\text{CALIBRATION2} - \text{CALIBRATION1}}{(\text{CALIBRATION2\_PERIODS}) - 1} = \frac{(23133 - 2315)}{(10 - 1)} = 2313.11$$

$$\text{normLSB} = \frac{(\text{CLOCKperiod})}{(\text{calCount})} = \frac{(1/8\text{MHz})}{2313.11} = 5.40 * 10^{-11}$$

$$\text{TOF1} = (\text{TIME1})(\text{normLSB}) + (\text{CLOCK\_COUNT1})(\text{CLOCKperiod}) - (\text{TIME2})(\text{normLSB})$$

$$\text{TOF1} = (2147)(5.40 * 10^{-11}) + (3818)(1/8\text{MHz}) - (201)(5.40 * 10^{-11})$$

$$\text{TOF1} = 39.855\mu\text{s} \quad (3)$$

## Device Functional Modes (continued)

### 8.4.3 Timeout

For one STOP, the TDC performs the measurement by counting from the START signal to the STOP signal. If no STOP signal is received, either the Clock Counter or Coarse Counter will overflow and will generate an interrupt (see [Coarse and Clock Counters Overflow](#)). If no START signal is received, the timer waits indefinitely for a START signal to arrive.

For multiple STOPS, the TDC performs the measurement by counting from the START signal to the last STOP signal. All earlier STOP signals are captured and stored into the corresponding Measurement Results registers ([TIME1](#) to [TIME6](#), [CLOCK\\_COUNT1](#) to [CLOCK\\_COUNT5](#), [CALIBRATION1](#), [CALIBRATION2](#)). The minimum time required between two consecutive STOP signals is defined in the [Recommended Operating Conditions](#) table. The device can be programmed to measure up to 5 STOP signals by setting the NUM\_STOP bits in the [CONFIG2](#) register.


### 8.4.4 Multi-Cycle Averaging

In the Multi-Cycle Averaging Mode, the TDC7200 will perform a series of measurements on its own and will only send an interrupt to the MCU (for example, MSP430, C2000, etc) for wake up after the series has been completed. While waiting, the MCU can remain in sleep mode during the whole cycle (as shown in [Figure 19](#)).

Multi-Cycle Averaging Mode Setup and Conditions:

- The number of averaging cycles should be selected (1 to 128). This is done by programming the AVG\_CYCLES bit in the [CONFIG2](#) register.
- The results of all measurements are reported in the Measurement Results registers ([TIME1](#) to [TIME6](#), [CLOCK\\_COUNT1](#) to [CLOCK\\_COUNT5](#), [CALIBRATION1](#), [CALIBRATION2](#) registers). The CLOCK\_COUNTn registers should be right shifted by the  $\log_2(\text{AVG\_CYCLES})$  before calculating the time-of-flight (TOF). For example, if using the multi-cycle averaging mode, [Equation 2](#) should be rewritten as:  $\text{TOFn} = \text{normLSB} [\text{TIME1} - \text{TIME}(n+1)] + [\text{CLOCK\_COUNTn} \gg \log_2(\text{AVG\_CYCLES})] \times [\text{CLOCKperiod}]$
- Following each average cycle, the TDC generates either a trigger event on the TRIGG pin after the calibration measurement to commence a new measurement or an interrupt on the INTB pin, indicating that the averaging sequence has completed.

This mode allows multiple measurements without MCU interaction, thus optimizing power consumption for the overall system.

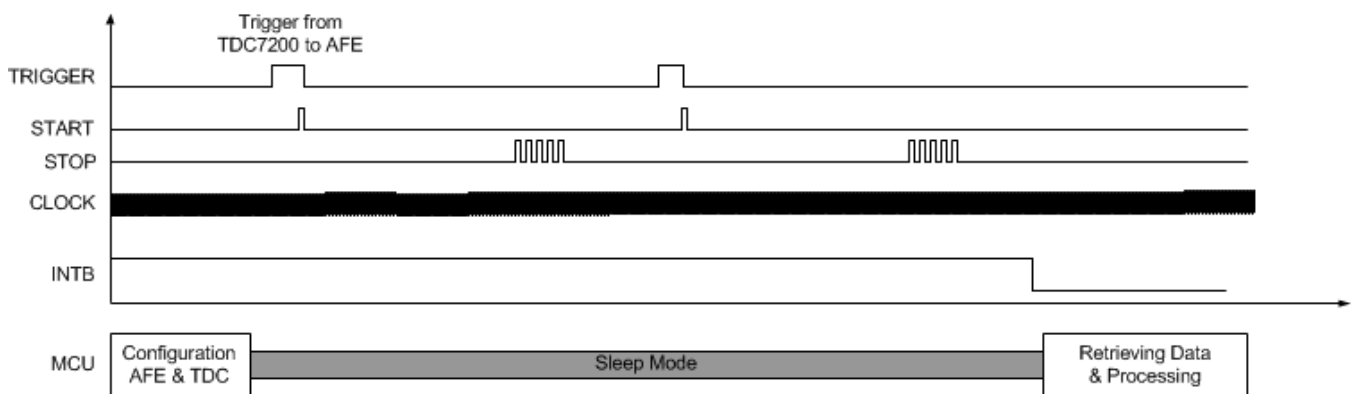

**Figure 19. Multi-Cycle Averaging Mode Example with 2 Averaging Cycles and 5 STOP Signals**

### 8.4.5 START and STOP Edge Polarity

In order to achieve the highest measurement accuracy, having the same edge polarity for the START and STOP input signals is highly recommended. Otherwise, slightly different propagation delays due to symmetry shift between the rising and falling edge configuration will impact the measurement accuracy.

For highest measurement accuracy in measurement mode 2, it's strongly recommended to choose for the START and STOP signal the "rising edge". This is done by setting the START\_EDGE and STOP\_EDGE bits in the [CONFIG1](#) register to 0.

## Device Functional Modes (continued)

### 8.4.6 Measurement Sequence


The TDC7200 is a stopwatch IC that measures time between a START and multiple STOP events. The measurement sequence of the TDC7200 is as follows:

1. After powering up the device, the EN pin needs to be low. There is one low to high transition required while VDD is supplied for correct initialization of the device.
2. MCU software requests a new measurement to be initiated via the SPI™ interface.
3. After the start new measurement bit START\_MEAS has been set in the [CONFIG1](#) register, the TDC7200 generates a trigger signal on the TRIGG pin, which is typically used by the corresponding ultrasonic analog-front-end (such as the TDC1000) as start trigger for a measurement (for example, transmit signal for the ultrasonic burst)
4. Immediately after sending the trigger, the TDC7200 enables the START pin and waits to receive the START pulse edge
5. After receiving a START, the TDC resets the TRIGG pin
6. The Clock counter is started after the next rising edge of the external clock signal (Measurement Mode 2). The Clock Counter STOP Mask registers ([CLOCK\\_CNTR\\_STOP\\_MASK\\_H](#) and [CLOCK\\_CNTR\\_STOP\\_MASK\\_L](#)) determine the length of the STOP mask window.
7. After reaching the Clock Counter STOP Mask value, the STOP pin waits to receive a single or multiple STOP trigger signal from the analog-front-end (for example, detected echo signal of the ultrasonic burst signal)
8. After the last STOP trigger has been received, the TDC will signal to the MCU via interrupt (INTB pin) that there are new measurement results waiting in the registers. START, STOP and TRIGG pin are disabled (in Multi-Cycle Averaging Mode, the TDC will start the next cycle automatically by generating a new TRIGG signal). Note: INTB must be utilized to determine TDC measurement completion; polling the [INT\\_STATUS](#) register to determine measurement completion is NOT recommended as it will interfere with the TDC measurement.
9. After the results are retrieved, the MCU can then start a new measurement with the same register settings. This is done by just setting the START measurement bit via SPI. It is not required to drive the ENABLE pin low between measurements.
10. The ENABLE pin can be taken low, if the time duration between measurements is long, and it is desired to put the TDC7200 in its lowest power state. However, upon taking ENABLE high again, the device will come up with its default register settings and will need to be configured via SPI.

### 8.4.7 Wait Times for TDC7200 Startup

The required wait time following the rising edge of the ENABLE pin of the TDC7200 is defined by three key times, as shown in [Figure 20](#). All three times relate to the startup of the TDC7200's internal LDO, which is power gated when the device is disabled for optimal power consumption. The first parameter,  $T1_{SPI\_RDY}$ , is the time after which the SPI interface is accessible. The second ( $T2_{LDO\_SET1}$ ) parameter and third ( $T3_{LDO\_SET2}$ ) parameter are related to the performance of a measurement made while the internal LDO is settling. The LDO supplies the TDC7200's time measurement device, and a change in voltage on its supply during a measurement translates directly to an inaccuracy. It is therefore recommended to wait until the LDO is settled before time measurement begins.

The first time period relating to the measurement accuracy is  $T2_{LDO\_SET1}$ , the LDO settling time 1. This is the time after which the LDO has settled to within 0.3% of its final value. A 0.3% error translates to a worst case time error (due to the LDO settling) of  $0.3\% \times t_{CLOCK}$ , which is 375ps in the case of an 8MHz reference clock, or 187.5ps if a 16MHz clock is used. Finally, the time  $T3_{LDO\_SET2}$  is the time after which the LDO has settled to its final value. For best performance, it is recommended that a time measurement is not started before  $T3_{LDO\_SET2}$  to allow the LDO to fully settle. Typical times for  $T1_{SPI\_RDY}$  is 100  $\mu$ s, for  $T2_{LDO\_SET1}$  is 300  $\mu$ s, and for  $T3_{LDO\_SET2}$  is 1.5 ms.

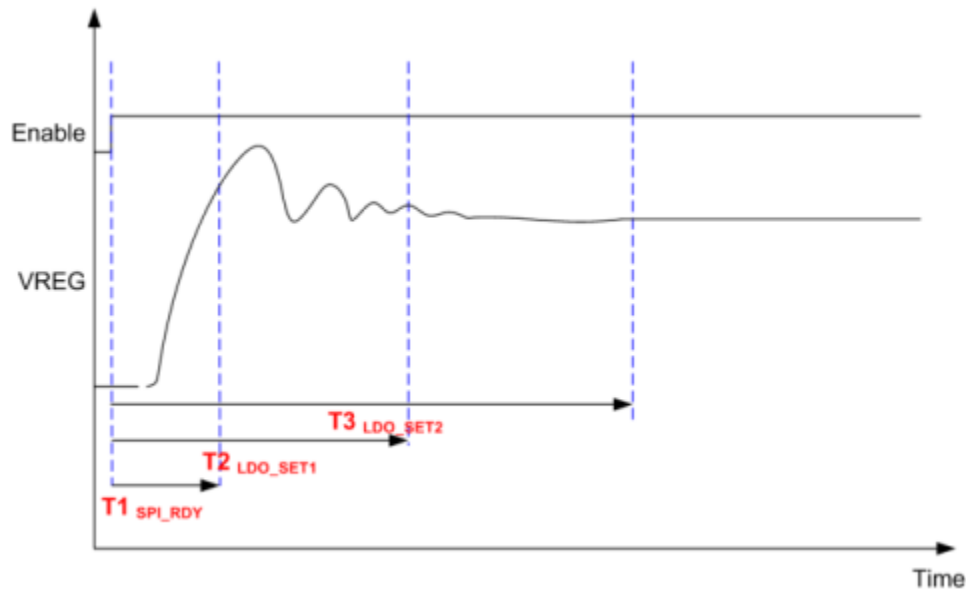**Device Functional Modes (continued)**

**Figure 20. VREG Startup Time**

## 8.5 Programming

### 8.5.1 Serial Peripheral Interface (SPI)

The serial interface consists of data input (DIN), data output (DOUT), serial interface clock (SCLK), and chip select bar (CSB). The serial interface is used to configure the TDC7200 parameters available in various configuration registers.

The communication on the SPI bus supports write and read transactions. A write transaction consists of a single write command byte, followed by single data byte. A read transaction consists of a single read command byte followed by 8 or 24 SCLK cycles. The write and read command bytes consist of a 1-bit auto-increment bit, a 1-bit read or write instruction, and a 6-bit register address. [Figure 21](#) shows the SPI protocol for a transaction involving one byte of data (read or write).

## Programming (continued)

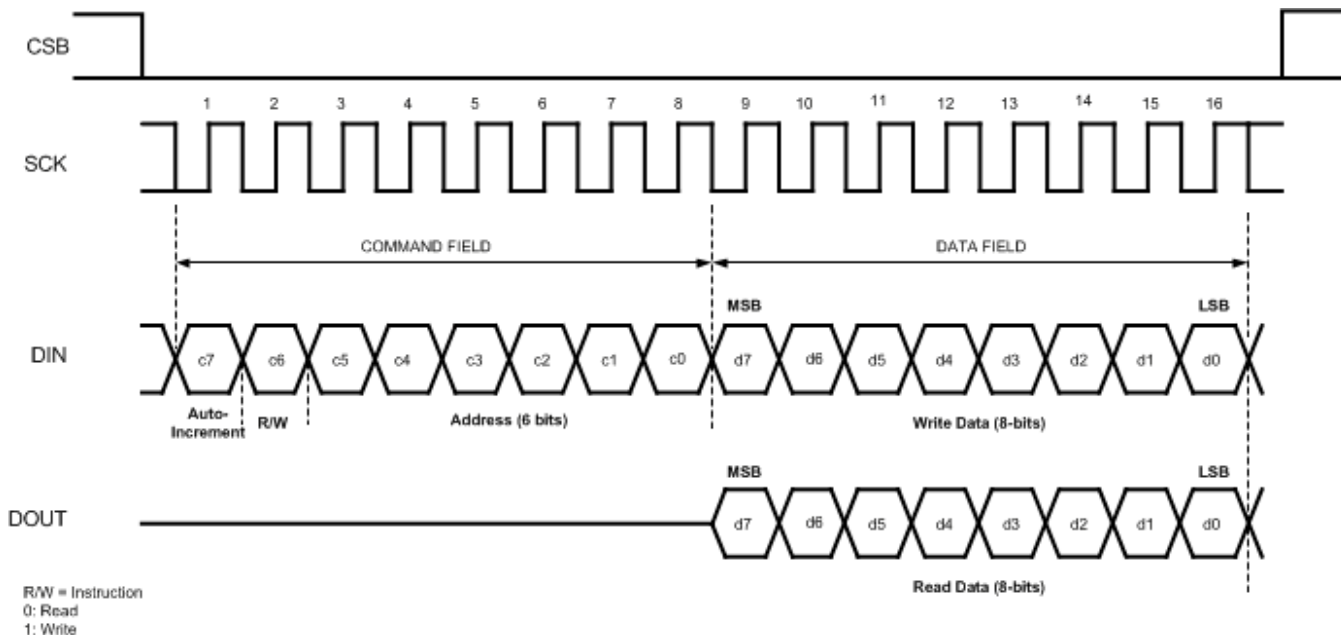


Figure 21. SPI Protocol

### 8.5.1.1 CSB

CSB is an active-low signal and needs to be low throughout a transaction. That is, CSB should not pulse between the command byte and the data byte of a single transaction.

De-asserting CSB always terminates an ongoing transaction, even if it is not yet complete. Re-asserting CSB will always bring the device into a state ready for the next transaction, regardless of the termination status of a previous transaction.

### 8.5.1.2 SCLK

SPI clock can idle high or low. It is recommended to keep SCLK as clean as possible to prevent glitches from corrupting the SPI frame.

### 8.5.1.3 DIN

Data In (DIN) is driven by the SPI master by sending the command and the data byte to configure the TDC7200.

### 8.5.1.4 DOUT

Data Out (DOUT) is driven by the TDC7200 when the SPI master initiates a read transaction. When the TDC7200 is not being read out, the DOUT pin is in high impedance mode and is undriven.

## Programming (continued)

### 8.5.1.5 Register Read/Write

Access to the internal registers can be done through the serial interface formed by pins CSB (Chip Select - active low), SCLK (serial interface clock), DIN (data input), and DOUT (data out).

Serial shift of bits into the device is enabled when CSB is low. Serial data DIN is latched (MSB received first, LSB received last) at every rising edge of SCLK when CSB is active (low). The serial data is loaded into the register with the last data bit SCLK rising edge when CSB is low. In the case that the word length exceeds the register size, the excess bits are ignored. The interface can work with SCLK frequency from 20MHz down to very low speeds (a few Hertz) and even with a non-50% duty-cycle SCLK.

The SPI transaction is divided in two main portions:

- Address and Control: Auto Increment Mode selection bit, Read/Write bit, Address 6 bits
- Data: 8 bit or 24 bit

When writing to a register with unused bits, these should be set to 0.

| Address and Control (A7 - A0) |                       |                  |    |    |    |    |    |
|-------------------------------|-----------------------|------------------|----|----|----|----|----|
| A7                            | A6                    | A5               | A4 | A3 | A2 | A1 | A0 |
| Auto Increment                | RW                    | Register Address |    |    |    |    |    |
| 0: OFF<br>1: ON               | Read = 0<br>Write = 1 | 00 h up to 3Fh   |    |    |    |    |    |

### 8.5.1.6 Auto Increment Mode

When the Auto Increment Mode is OFF, only the register indicated by the Register Address will be accessed, all cycles beyond the register length will be ignored. When the Auto Increment is ON, the register of the Register Address is accessed first, then without interruption, subsequent registers are accessed.

The Auto Increment Mode can be either used to access the configuration ([CONFIG1](#) and [CONFIG2](#)) and status ([INT\\_STATUS](#)) registers, or for the Measurement Results registers ([TIME1](#) to [TIME6](#), [CLOCK\\_COUNT1](#) to [CLOCK\\_COUNT5](#), [CALIBRATION1](#), [CALIBRATION2](#)). As both register block use registers with different length, it's not possible to access all registers of the device within one single access cycle.

## 8.6 Register Maps

### 8.6.1 Register Initialization

After power up (VDD supplied, ENABLE Pin low to high transition) the internal registers are initialized with the default value. Disabling the part by pulling ENABLE pin to GND will set the device into total shutdown. As the internal LDO is turned off settings in the register will be lost. The device initializes the registers with default values with the next enable (ENABLE pin to VDD).

**Table 1. Register Summary**

| REGISTER ADDRESS | REGISTER NAME          | REGISTER DESCRIPTION                    | SIZE (BITS) | RESET VALUE |
|------------------|------------------------|---|-------------|-------------|
| 00h              | CONFIG1                | Configuration Register 1                | 8           | 00h         |
| 01h              | CONFIG2                | Configuration Register 2                | 8           | 40h         |
| 02h              | INT_STATUS             | Interrupt Status Register               | 8           | 00h         |
| 03h              | INT_MASK               | Interrupt Mask Register                 | 8           | 07h         |
| 04h              | COARSE_CNTR_OVF_H      | Coarse Counter Overflow Value High      | 8           | FFh         |
| 05h              | COARSE_CNTR_OVF_L      | Coarse Counter Overflow Value Low       | 8           | FFh         |
| 06h              | CLOCK_CNTR_OVF_H       | CLOCK Counter Overflow Value High       | 8           | FFh         |
| 07h              | CLOCK_CNTR_OVF_L       | CLOCK Counter Overflow Value Low        | 8           | FFh         |
| 08h              | CLOCK_CNTR_STOP_MASK_H | CLOCK Counter STOP Mask High            | 8           | 00h         |
| 09h              | CLOCK_CNTR_STOP_MASK_L | CLOCK Counter STOP Mask Low             | 8           | 00h         |
| 10h              | TIME1                  | Measured Time 1                         | 24          | 00_0000h    |
| 11h              | CLOCK_COUNT1           | CLOCK Counter Value                     | 24          | 00_0000h    |
| 12h              | TIME2                  | Measured Time 2                         | 24          | 00_0000h    |
| 13h              | CLOCK_COUNT2           | CLOCK Counter Value                     | 24          | 00_0000h    |
| 14h              | TIME3                  | Measured Time 3                         | 24          | 00_0000h    |
| 15h              | CLOCK_COUNT3           | CLOCK Counter Value                     | 24          | 00_0000h    |
| 16h              | TIME4                  | Measured Time 4                         | 24          | 00_0000h    |
| 17h              | CLOCK_COUNT4           | CLOCK Counter Value                     | 24          | 00_0000h    |
| 18h              | TIME5                  | Measured Time 5                         | 24          | 00_0000h    |
| 19h              | CLOCK_COUNT5           | CLOCK Counter Value                     | 24          | 00_0000h    |
| 1Ah              | TIME6                  | Measured Time 6                         | 24          | 00_0000h    |
| 1Bh              | CALIBRATION1           | Calibration 1, 1 CLOCK Period           | 24          | 00_0000h    |
| 1Ch              | CALIBRATION2           | Calibration 2, 2/10/20/40 CLOCK Periods | 24          | 00_0000h    |

**8.6.2 CONFIG1: Configuration Register 1 R/W (address = 00h) [reset = 0h]**
**Figure 22. Configuration Register 1**

| 7         | 6         | 5          | 4         | 3          | 2         | 1      | 0          |
|-----------|-----------|------------|-----------|------------|-----------|--------|------------|
| FORCE_CAL | PARITY_EN | TRIGG_EDGE | STOP_EDGE | START_EDGE | MEAS_MODE |        | START_MEAS |
| R/W-0h    | R/W-0h    | R/W-0h     | R/W-0h    | R/W-0h     | R/W-0h    | R/W-0h | R/W-0h     |

LEGEND: R/W = Read/Write; R = Read only; -n = value after reset

**Table 2. Configuration Register 1 Field Descriptions**

| Bit   | Field      | Type | Reset | Description  |
|-------|------------|------|-------|--|
| 7     | FORCE_CAL  | R/W  | 0     | 0: Calibration is not performed after interrupted measurement (for example, due to counter overflow or missing STOP signal)<br>1: Calibration is always performed at the end (for example, after a counter overflow)   |
| 6     | PARITY_EN  | R/W  | 0     | 0: Parity bit for Measurement Result Registers* disabled (Parity Bit always 0)<br>1: Parity bit for Measurement Result Registers enabled (Even Parity)<br>*The Measurement Results registers are the <a href="#">TIME1</a> to <a href="#">TIME6</a> , <a href="#">CLOCK_COUNT1</a> to <a href="#">CLOCK_COUNT5</a> , <a href="#">CALIBRATION1</a> , <a href="#">CALIBRATION2</a> registers.  |
| 5     | TRIGG_EDGE | R/W  | 0     | 0: TRIGG is output as a Rising edge signal<br>1: TRIGG is output as a Falling edge signal  |
| 4     | STOP_EDGE  | R/W  | 0     | 0: Measurement is stopped on Rising edge of STOP signal<br>1: Measurement is stopped on Falling edge of STOP signal  |
| 3     | START_EDGE | R/W  | 0     | 0: Measurement is started on Rising edge of START signal<br>1: Measurement is started on Falling edge of START signal  |
| [2:1] | MEAS_MODE  | R/W  | 00h   | 00: Measurement Mode 1 (for expected time-of-flight < 500 ns).<br>01: Measurement Mode 2 (recommended)<br>10, 11: Reserved for future functionality  |
| 0     | START_MEAS | R/W  | 0     | Start New Measurement:<br>This bit is cleared when Measurement is Completed.<br>0: No effect<br>1: Start New Measurement. Writing a 1 will clear all bits in the Interrupt Status Register and Start the measurement (by generating an TRIGG signal) and will reset the content of all Measurement Results registers ( <a href="#">TIME1</a> to <a href="#">TIME6</a> , <a href="#">CLOCK_COUNT1</a> to <a href="#">CLOCK_COUNT5</a> , <a href="#">CALIBRATION1</a> , <a href="#">CALIBRATION2</a> ) to 0. |

**8.6.3 CONFIG2: Configuration Register 2 R/W (address = 01h) [reset = 40h]**
**Figure 23. Configuration Register 2**

| 7                    | 6      | 5          | 4      | 3      | 2        | 1      | 0      |
|----------------------|--------|------------|--------|--------|----------|--------|--------|
| CALIBRATION2_PERIODS |        | AVG_CYCLES |        |        | NUM_STOP |        |        |
| R/W-0h               | R/W-1h | R/W-0h     | R/W-0h | R/W-0h | R/W-0h   | R/W-0h | R/W-0h |

LEGEND: R/W = Read/Write; R = Read only; -n = value after reset

**Table 3. Configuration Register 2 Field Descriptions**

| Bit   | Field                | Type | Reset | Description   |
|-------|----------------------|------|-------|---|
| [7:6] | CALIBRATION2_PERIODS | R/W  | 01h   | 00: Calibration 2 - measuring 2 CLOCK periods<br>01: Calibration 2 - measuring 10 CLOCK periods<br>10: Calibration 2 - measuring 20 CLOCK periods<br>11: Calibration 2 - measuring 40 CLOCK periods   |
| [5:3] | AVG_CYCLES           | R/W  | 00h   | 000: 1 Measurement Cycle only (no Multi-Cycle Averaging Mode)<br>001: 2 Measurement Cycles<br>010: 4 Measurement Cycles<br>011: 8 Measurement Cycles<br>100: 16 Measurement Cycles<br>101: 32 Measurement Cycles<br>110: 64 Measurement Cycles<br>111: 128 Measurement Cycles |
| [2:0] | NUM_STOP             | R/W  | 00h   | 000: Single Stop<br>001: Two Stops<br>010: Three Stops<br>011: Four Stops<br>100: Five Stops<br>101, 110, 111: No Effect. Single Stop   |

**8.6.4 INT\_STATUS: Interrupt Status Register (address = 02h) [reset = 00h]**
**Figure 24. Interrupt Status Register**

| 7        | 6        | 5        | 4                  | 3                 | 2                      | 1                        | 0            |
|----------|----------|----------|--------------------|-------------------|------------------------|--------------------------|--------------|
| Reserved | Reserved | Reserved | MEAS_COMPLETE_FLAG | MEAS_STARTED_FLAG | CLOCK_CNT_OVERFLOW_INT | COARSE_CNTR_OVERFLOW_INT | NEW_MEAS_INT |
| R/W-0h   | R/W-0h   | R/W-0h   | R/W-0h             | R/W-0h            | R/W-0h                 | R/W-0h                   | R/W-0h       |

LEGEND: R/W = Read/Write; R = Read only; -n = value after reset

**Table 4. Interrupt Status Register Field Descriptions**

| Bit | Field                    | Type | Reset | Description   |
|-----|--------------------------|------|-------|---|
| 7   | Reserved                 | R/W  | 0h    |   |
| 6   | Reserved                 | R/W  | 0h    |   |
| 5   | Reserved                 | R/W  | 0h    |   |
| 4   | MEAS_COMPLETE_FLAG       | R/W  | 0h    | Writing a 1 will clear the status<br>0: Measurement has not completed<br>1: Measurement has completed (same information as NEW_MEAS_INT)                  |
| 3   | MEAS_STARTED_FLAG        | R/W  | 0h    | Writing a 1 will clear the status<br>0: Measurement has not started<br>1: Measurement has started (START signal received)                                 |
| 2   | CLOCK_CNTR_OVERFLOW_INT  | R/W  | 0h    | Requires writing a 1 to clear interrupt status<br>0: No overflow detected<br>1: Clock overflow detected, running measurement will be stopped immediately  |
| 1   | COARSE_CNTR_OVERFLOW_INT | R/W  | 0h    | Requires writing a 1 to clear interrupt status<br>0: No overflow detected<br>1: Coarse overflow detected, running measurement will be stopped immediately |
| 0   | NEW_MEAS_INT             | R/W  | 0h    | Requires writing a 1 to clear interrupt status<br>0: Interrupt not detected<br>1: Interrupt detected – New Measurement has been completed                 |

**8.6.5 INT\_MASK: Interrupt Mask Register R/W (address = 03h) [reset = 07h]**
**Figure 25. Interrupt Mask Register**

| 7       | 6       | 5       | 4       | 3       | 2                   | 1                    | 0             |
|---------|---------|---------|---------|---------|---------------------|----------------------|---------------|
| Reserve | Reserve | Reserve | Reserve | Reserve | CLOCK_CNTR_OVF_MASK | COARSE_CNTR_OVF_MASK | NEW_MEAS_MASK |
| R/W-0h  | R/W-0h  | R/W-0h  | R/W-0h  | R/W-0h  | R/W-1h              | R/W-1h               | R/W-1h        |

LEGEND: R/W = Read/Write; R = Read only; -n = value after reset

**Table 5. Interrupt Mask Register Field Descriptions**

| Bit | Field                | Type | Reset | Description   |
|-----|----------------------|------|-------|---|
| 7   | Reserve              | R/W  | 0     |   |
| 6   | Reserve              | R/W  | 0     |   |
| 5   | Reserve              | R/W  | 0     |   |
| 4   | Reserve              | R/W  | 0     |   |
| 3   | Reserve              | R/W  | 0     |   |
| 2   | CLOCK_CNTR_OVF_MASK  | R/W  | 1     | 0: CLOCK Counter Overflow Interrupt disabled<br>1: CLOCK Counter Overflow Interrupt enabled   |
| 1   | COARSE_CNTR_OVF_MASK | R/W  | 1     | 0: Coarse Counter Overflow Interrupt disabled<br>1: Coarse Counter Overflow Interrupt enabled |
| 0   | NEW_MEAS_MASK        | R/W  | 1     | 0: New Measurement Interrupt disabled<br>1: New Measurement Interrupt enabled                 |

A disabled interrupt will no longer be visible on the device pin (INTB). The interrupt bit in the [INT\\_STATUS](#) register will still be active.

**8.6.6 COARSE\_CNTR\_OVF\_H: Coarse Counter Overflow High Value Register (address = 04h) [reset = FFh]**
**Figure 26. Coarse Counter Overflow Value\_H Register**

| 7                 | 6      | 5      | 4      | 3      | 2      | 1      | 0      |
|-------------------|--------|--------|--------|--------|--------|--------|--------|
| COARSE_CNTR_OVF_H |        |        |        |        |        |        |        |
| R/W-1h            | R/W-1h | R/W-1h | R/W-1h | R/W-1h | R/W-1h | R/W-1h | R/W-1h |

LEGEND: R/W = Read/Write; R = Read only; -n = value after reset

**Table 6. Coarse Counter Overflow Value\_H Register Field Descriptions**

| Bit | Field             | Type | Reset | Description                                |
|-----|-------------------|------|-------|--|
| 7-0 | COARSE_CNTR_OVF_H | R/W  | FFh   | Coarse Counter Overflow Value, upper 8 Bit |

**8.6.7 COARSE\_CNTR\_OVF\_L: Coarse Counter Overflow Low Value Register (address = 05h) [reset = FFh ]**
**Figure 27. Coarse Counter Overflow Value\_L Register**

| 7                 | 6      | 5      | 4      | 3      | 2      | 1      | 0      |
|-------------------|--------|--------|--------|--------|--------|--------|--------|
| COARSE_CNTR_OVF_L |        |        |        |        |        |        |        |
| R/W-1h            | R/W-1h | R/W-1h | R/W-1h | R/W-1h | R/W-1h | R/W-1h | R/W-1h |

LEGEND: R/W = Read/Write; R = Read only; -n = value after reset

**Table 7. Coarse Counter Overflow Value\_L Register Field Descriptions**

| Bit | Field             | Type | Reset | Description   |
|-----|-------------------|------|-------|---|
| 7-0 | COARSE_CNTR_OVF_L | R/W  | FFh   | Coarse Counter Overflow Value, lower 8 Bit<br>Note: Don't set COARSE_CNTR_OVF_L to 1. |

**8.6.8 CLOCK\_CNTR\_OVF\_H: Clock Counter Overflow High Register (address = 06h) [reset = FFh]**
**Figure 28. CLOCK Counter Overflow Value\_H Register**

| 7                | 6      | 5      | 4      | 3      | 2      | 1      | 0      |
|------------------|--------|--------|--------|--------|--------|--------|--------|
| CLOCK_CNTR_OVF_H |        |        |        |        |        |        |        |
| R/W-1h           | R/W-1h | R/W-1h | R/W-1h | R/W-1h | R/W-1h | R/W-1h | R/W-1h |

LEGEND: R/W = Read/Write; R = Read only; -n = value after reset

**Table 8. CLOCK Counter Overflow Value\_H Register Field Descriptions**

| Bit | Field            | Type | Reset | Description                               |
|-----|------------------|------|-------|---|
| 7-0 | CLOCK_CNTR_OVF_H | R/W  | FFh   | CLOCK Counter Overflow Value, upper 8 Bit |

**8.6.9 CLOCK\_CNTR\_OVF\_L: Clock Counter Overflow Low Register (address = 07h) [reset = FFh]**
**Figure 29. CLOCK Counter Overflow Value\_L Register**

| 7                | 6      | 5      | 4      | 3      | 2      | 1      | 0      |
|------------------|--------|--------|--------|--------|--------|--------|--------|
| CLOCK_CNTR_OVF_L |        |        |        |        |        |        |        |
| R/W-1h           | R/W-1h | R/W-1h | R/W-1h | R/W-1h | R/W-1h | R/W-1h | R/W-1h |

LEGEND: R/W = Read/Write; R = Read only; -n = value after reset

**Table 9. CLOCK Counter Overflow Value\_L Register Field Descriptions**

| Bit | Field            | Type | Reset | Description                               |
|-----|------------------|------|-------|---|
| 7-0 | CLOCK_CNTR_OVF_L | R/W  | FFh   | CLOCK Counter Overflow Value, lower 8 Bit |

**8.6.10 CLOCK\_CNTR\_STOP\_MASK\_H: CLOCK Counter STOP Mask High Value Register (address = 08h)  
[reset = 00h]**
**Figure 30. CLOCK Counter STOP Mask\_H Register**

|                        |        |        |        |        |        |        |        |
|------------------------|--------|--------|--------|--------|--------|--------|--------|
| 7                      | 6      | 5      | 4      | 3      | 2      | 1      | 0      |
| CLOCK_CNTR_STOP_MASK_H |        |        |        |        |        |        |        |
| R/W-0h                 | R/W-0h | R/W-0h | R/W-0h | R/W-0h | R/W-0h | R/W-0h | R/W-0h |

LEGEND: R/W = Read/Write; R = Read only; -n = value after reset

**Table 10. CLOCK Counter STOP Mask\_H Register Field Descriptions**

| Bit | Field                  | Type | Reset | Description                          |
|-----|------------------------|------|-------|--------------------------------------|
| 7-0 | CLOCK_CNTR_STOP_MASK_H | R/W  | 0     | CLOCK Counter STOP Mask, upper 8 Bit |

**8.6.11 CLOCK\_CNTR\_STOP\_MASK\_L: CLOCK Counter STOP Mask Low Value Register (address = 09h)  
[reset = 00h]**
**Figure 31. CLOCK Counter STOP Mask\_L Register**

|                        |        |        |        |        |        |        |        |
|------------------------|--------|--------|--------|--------|--------|--------|--------|
| 7                      | 6      | 5      | 4      | 3      | 2      | 1      | 0      |
| CLOCK_CNTR_STOP_MASK_L |        |        |        |        |        |        |        |
| R/W-0h                 | R/W-0h | R/W-0h | R/W-0h | R/W-0h | R/W-0h | R/W-0h | R/W-0h |

LEGEND: R/W = Read/Write; R = Read only; -n = value after reset

**Table 11. CLOCK Counter STOP Mask\_L Register Field Descriptions**

| Bit | Field                  | Type | Reset | Description                          |
|-----|------------------------|------|-------|--------------------------------------|
| 7-0 | CLOCK_CNTR_STOP_MASK_L | R/W  | 0     | CLOCK Counter STOP Mask, lower 8 Bit |

**8.6.12 TIME1: Time 1 Register (address: 10h) [reset = 00\_0000h]**
**Figure 32. TIME1 Register**

|            |  |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |
|------------|--|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|
| 23         | 22   | 21  | 20  | 19  | 18  | 17  | 16  | 15  | 14  | 13  | 12  | 11  | 10  | 9   | 8   | 7   | 6   | 5   | 4   | 3   | 2   | 1   | 0   |
| Parity Bit | Measurement Result: 23 bit integer value (Bit 22: MSB, Bit 0: LSB) |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |
| R-0        | R-0  | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 |

LEGEND: R/W = Read/Write; R = Read only; -n = value after reset

**Table 12. TIME1 Register Field Descriptions**

| Bit  | Field  | Type | Reset | Description        |
|------|--|------|-------|--------------------|
| 23   | Parity Bit   | R    | 0     | Parity Bit         |
| 22-0 | Measurement Result: 23 bit integer value (Bit 22: MSB, Bit 0: LSB) | R    | 0     | Measurement Result |

**8.6.13 CLOCK\_COUNT1: Clock Count Register (address: 11h) [reset = 00\_0000h]**

**Figure 33. CLOCK Count Register**

|            |                     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |
|------------|---------------------|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|
| 23         | 22                  | 21  | 20  | 19  | 18  | 17  | 16  | 15  | 14  | 13  | 12  | 11  | 10  | 9   | 8   | 7   | 6   | 5   | 4   | 3   | 2   | 1   | 0   |
| Parity Bit | CLOCK_COUNT1 Result |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |
| R-0        | R-0                 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 |

LEGEND: R/W = Read/Write; R = Read only; -n = value after reset

**Table 13. CLOCK\_COUNT1 Register Field Descriptions**

| Bit   | Field                           | Type | Reset | Description   |
|-------|---------------------------------|------|-------|---|
| 23    | Parity Bit                      | R    | 0     | Parity Bit  |
| 22-16 | Not Used                        | R    | 0     | These bits will be used in Multi-Cycle Averaging Mode in order to allow higher averaging results. |
| 15-0  | CLOCK_COUNT1 Measurement Result | R    | 0     | CLOCK_COUNT1 Measurement Result   |

**8.6.14 TIME2: Time 2 Register (address: 12h) [reset = 00\_0000h]**

**Figure 34. TIME2 Register**

|            |  |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |
|------------|--|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|
| 23         | 22   | 21  | 20  | 19  | 18  | 17  | 16  | 15  | 14  | 13  | 12  | 11  | 10  | 9   | 8   | 7   | 6   | 5   | 4   | 3   | 2   | 1   | 0   |
| Parity Bit | Measurement Result: 23 bit integer value (Bit 22: MSB, Bit 0: LSB) |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |
| R-0        | R-0  | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 |

LEGEND: R/W = Read/Write; R = Read only; -n = value after reset

**Table 14. TIME2 Register Field Descriptions**

| Bit  | Field              | Type | Reset | Description        |
|------|--------------------|------|-------|--------------------|
| 23   | Parity Bit         | R    | 0     | Parity Bit         |
| 22-0 | Measurement Result | R    | 0     | Measurement Result |

**8.6.15 CLOCK\_COUNT2: Clock Count Register (address: 13h) [reset = 00\_0000h]**

**Figure 35. CLOCK\_COUNT2 Register**

|            |              |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |
|------------|--------------|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|
| 23         | 22           | 21  | 20  | 19  | 18  | 17  | 16  | 15  | 14  | 13  | 12  | 11  | 10  | 9   | 8   | 7   | 6   | 5   | 4   | 3   | 2   | 1   | 0   |
| Parity Bit | CLOCK_COUNT2 |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |
| R-0        | R-0          | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 |

LEGEND: R/W = Read/Write; R = Read only; -n = value after reset

**Table 15. CLOCK\_COUNT2 Register Field Descriptions**

| Bit   | Field               | Type | Reset | Description   |
|-------|---------------------|------|-------|---|
| 23    | Parity bit          | R    | 0     | Parity Bit  |
| 22-16 | Not Used            | R    | 0     | These bits will be used in Multi-Cycle Averaging Mode in order to allow higher averaging results. |
| 15-0  | CLOCK_COUNT2 result | R    | 0     | CLOCK_COUNT2 result   |

**8.6.16 TIME3: Time 3 Register (address: 14h) [reset = 00\_0000h]**
**Figure 36. TIME3 Register**

|            |  |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |
|------------|--|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|
| 23         | 22   | 21  | 20  | 19  | 18  | 17  | 16  | 15  | 14  | 13  | 12  | 11  | 10  | 9   | 8   | 7   | 6   | 5   | 4   | 3   | 2   | 1   | 0   |     |
| Parity Bit | Measurement Result: 23 bit integer value (Bit 22: MSB, Bit 0: LSB) |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |
| R-0        | R-0  | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 |

LEGEND: R/W = Read/Write; R = Read only; -n = value after reset

**Table 16. TIME3 Register Field Descriptions**

| Bit  | Field              | Type | Reset | Description        |
|------|--------------------|------|-------|--------------------|
| 23   | Parity bit         | R    | 0     | Parity Bit         |
| 22-0 | Measurement result | R    | 0     | Measurement Result |

**8.6.17 CLOCK\_COUNT3: Clock Count Registers (address: 15h) [reset = 00\_0000h]**
**Figure 37. CLOCK\_COUNT3 Count Register**

|            |              |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |
|------------|--------------|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|
| 23         | 22           | 21  | 20  | 19  | 18  | 17  | 16  | 15  | 14  | 13  | 12  | 11  | 10  | 9   | 8   | 7   | 6   | 5   | 4   | 3   | 2   | 1   | 0   |     |
| Parity Bit | CLOCK_COUNT3 |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |
| R-0        | R-0          | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 |

LEGEND: R/W = Read/Write; R = Read only; -n = value after reset

**Table 17. CLOCK\_COUNT3 Register Field Descriptions**

| Bit   | Field               | Type | Reset | Description   |
|-------|---------------------|------|-------|---|
| 23    | Parity bit          | R    | 0     | Parity bit  |
| 22-16 | Not Used            | R    | 0     | These bits will be used in Multi-Cycle Averaging Mode in order to allow higher averaging results. |
| 15-0  | CLOCK_COUNT3 Result | R    | 0     | CLOCK_COUNT3 Result   |

**8.6.18 TIME4: Time 4 Register (address: 16h) [reset = 00\_0000h]**
**Figure 38. TIME4 Register**

|            |  |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |
|------------|--|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|
| 23         | 22   | 21  | 20  | 19  | 18  | 17  | 16  | 15  | 14  | 13  | 12  | 11  | 10  | 9   | 8   | 7   | 6   | 5   | 4   | 3   | 2   | 1   | 0   |     |
| Parity Bit | Measurement Result: 23 bit integer value (Bit 22: MSB, Bit 0: LSB) |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |
| R-0        | R-0  | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 |

LEGEND: R/W = Read/Write; R = Read only; -n = value after reset

**Table 18. TIME4 Register Field Descriptions**

| Bit  | Field              | Type | Reset | Description        |
|------|--------------------|------|-------|--------------------|
| 23   | Parity bit         | R    | 0     |                    |
| 22-0 | Measurement result | R    | 0     | Measurement result |

**8.6.19 CLOCK\_COUNT4: Clock Count Register (address: 17h) [reset = 00\_0000h]**
**Figure 39. CLOCK\_COUNT4 Count Register**

|            |              |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |
|------------|--------------|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|
| 23         | 22           | 21  | 20  | 19  | 18  | 17  | 16  | 15  | 14  | 13  | 12  | 11  | 10  | 9   | 8   | 7   | 6   | 5   | 4   | 3   | 2   | 1   | 0   |
| Parity Bit | CLOCK_COUNT4 |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |
| R-0        | R-0          | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 |

LEGEND: R/W = Read/Write; R = Read only; -n = value after reset

**Table 19. CLOCK\_COUNT4 Register Field Descriptions**

| Bit   | Field               | Type | Reset | Description   |
|-------|---------------------|------|-------|---|
| 23    | Parity bit          | R    | 0     | Parity bit  |
| 22-16 | Not Used            | R    | 0     | These bits will be used in Multi-Cycle Averaging Mode in order to allow higher averaging results. |
| 15-0  | CLOCK_COUNT4 Result | R    | 0     | CLOCK_COUNT4 Result   |

**8.6.20 TIME5: Time 5 Register (address: 18h) [reset = 00\_0000h]**
**Figure 40. TIME5 Register**

|            |  |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |
|------------|--|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|
| 23         | 22   | 21  | 20  | 19  | 18  | 17  | 16  | 15  | 14  | 13  | 12  | 11  | 10  | 9   | 8   | 7   | 6   | 5   | 4   | 3   | 2   | 1   | 0   |
| Parity Bit | Measurement Result: 23 bit integer value (Bit 22: MSB, Bit 0: LSB) |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |
| R-0        | R-0  | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 |

LEGEND: R/W = Read/Write; R = Read only; -n = value after reset

**Table 20. TIME5 Register Field Descriptions**

| Bit  | Field              | Type | Reset | Description        |
|------|--------------------|------|-------|--------------------|
| 23   | Parity bit         | R    | 0     | Parity Bit         |
| 22-0 | Measurement result | R    | 0     | Measurement result |

**8.6.21 CLOCK\_COUNT5: Clock Count Register (address: 19h) [reset = 00\_0000h]**
**Figure 41. CLOCK\_COUNT5 Count Register**

|            |              |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |
|------------|--------------|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|
| 23         | 22           | 21  | 20  | 19  | 18  | 17  | 16  | 15  | 14  | 13  | 12  | 11  | 10  | 9   | 8   | 7   | 6   | 5   | 4   | 3   | 2   | 1   | 0   |
| Parity Bit | CLOCK_COUNT5 |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |
| R-0        | R-0          | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 |

LEGEND: R/W = Read/Write; R = Read only; -n = value after reset

**Table 21. CLOCK\_COUNT5 Register Field Descriptions**

| Bit   | Field               | Type | Reset | Description   |
|-------|---------------------|------|-------|---|
| 23    | Parity bit          | R    | 0     | Parity bit  |
| 22-16 | Not Used            | R    | 0     | These bits will be used in Multi-Cycle Averaging Mode in order to allow higher averaging results. |
| 15-0  | CLOCK_COUNT5 Result | R    | 0     | CLOCK_COUNT5 Result   |

**8.6.22 TIME6: Time 6 Register (address: 1Ah) [reset = 00\_0000h]**
**Figure 42. TIME6 Register**

|            |  |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |
|------------|--|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|
| 23         | 22   | 21  | 20  | 19  | 18  | 17  | 16  | 15  | 14  | 13  | 12  | 11  | 10  | 9   | 8   | 7   | 6   | 5   | 4   | 3   | 2   | 1   | 0   |     |
| Parity Bit | Measurement Result: 23 bit integer value (Bit 22: MSB, Bit 0: LSB) |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |
| R-0        | R-0  | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 |

LEGEND: R/W = Read/Write; R = Read only; -n = value after reset

**Table 22. TIME6 Register Field Descriptions**

| Bit  | Field              | Type | Reset | Description        |
|------|--------------------|------|-------|--------------------|
| 23   | Parity bit         | R    | 0     | Parity Bit         |
| 22-0 | Measurement result | R    | 0     | Measurement result |

**8.6.23 CALIBRATION1: Calibration 1 Register (address: 1Bh ) [reset = 00\_0000h]**
**Figure 43. CALIBRATION1 Register**

|            |              |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |
|------------|--------------|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|
| 23         | 22           | 21  | 20  | 19  | 18  | 17  | 16  | 15  | 14  | 13  | 12  | 11  | 10  | 9   | 8   | 7   | 6   | 5   | 4   | 3   | 2   | 1   | 0   |     |
| Parity Bit | CALIBRATION1 |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |
| R-0        | R-0          | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 |

LEGEND: R/W = Read/Write; R = Read only; -n = value after reset

**Table 23. CALIBRATION1 Register Field Descriptions**

| Bit  | Field        | Type | Reset | Description  |
|------|--------------|------|-------|--|
| 23   | Parity Bit   | R    | 0     | Parity Bit   |
| 22-0 | CALIBRATION1 | R    | 0     | Calibration 1 Result: 23 bit integer value (Bit 22: MSB, Bit 0: LSB) |

**8.6.24 CALIBRATION2: Calibration 2 Register (address: 1Ch ) [reset = 00\_0000h]**
**Figure 44. CALIBRATION2 Register**

|            |              |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |
|------------|--------------|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|
| 23         | 22           | 21  | 20  | 19  | 18  | 17  | 16  | 15  | 14  | 13  | 12  | 11  | 10  | 9   | 8   | 7   | 6   | 5   | 4   | 3   | 2   | 1   | 0   |     |
| Parity Bit | CALIBRATION2 |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |
| R-0        | R-0          | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 | R-0 |

LEGEND: R/W = Read/Write; R = Read only; -n = value after reset

**Table 24. CALIBRATION2 Register Field Descriptions**

| Bit  | Field        | Type | Reset | Description  |
|------|--------------|------|-------|--|
| 23   | Parity Bit   | R    | 0     | Parity Bit   |
| 22-0 | CALIBRATION2 | R    | 0     | Calibration 2 Result: 23 bit integer value (Bit 22: MSB, Bit 0: LSB) |

## 9 Application and Implementation

### NOTE

Information in the following applications sections is not part of the TI component specification, and TI does not warrant its accuracy or completeness. TI's customers are responsible for determining suitability of components for their purposes. Customers should validate and test their design implementation to confirm system functionality.

### 9.1 Application Information

In the Time Of Flight (TOF) method, the upstream flight time as well as the downstream flight time is measured. The difference between the Downstream and Upstream values is proportional to the flow.

The microcontroller (MCU) configures the TDC and AFE and issues a measurement start command to the TDC via the SPI interface. The TDC sends a TRIGGER pulse to the AFE which is set up to actuate one of the transducers and transmit a START signal to the TDC which starts its counter(s). The echo pulse will travel through the AFE and arrive to the TDC as the STOP signal. The counter will be stopped and after performing calibration, the counter value is reported as VAL.

Depending on system implementation, the above procedure is repeated for the same direction or opposite direction.

### 9.2 Typical Application

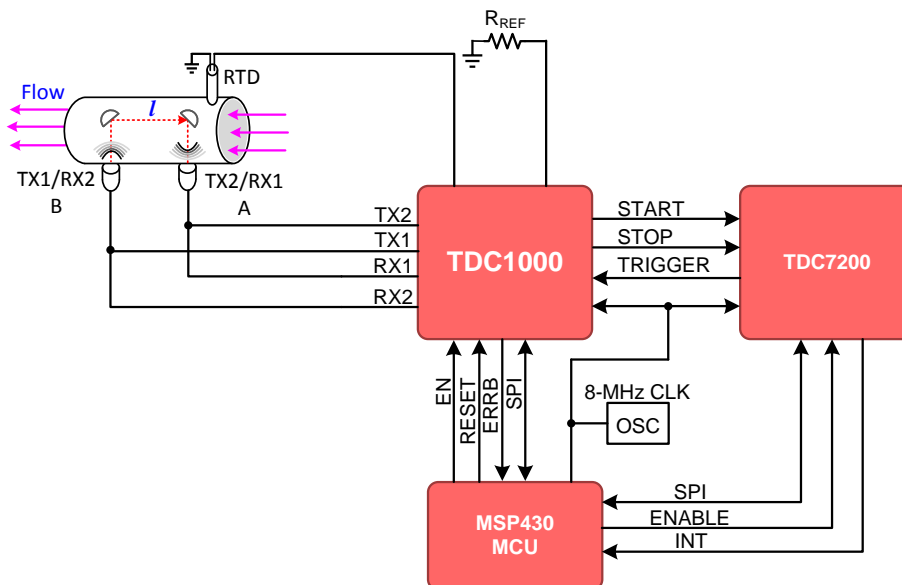


Figure 45. System in Time of Flight Mode

#### 9.2.1 Design Requirements

The parameters in this section are considered for this example.

Table 25. Design Parameters

| DESIGN PARAMETER              | EXAMPLE VALUE           |
|-------------------------------|-------------------------|
| Pipe diameter                 | 15 mm                   |
| Distance between transducers  | 60 mm                   |
| Minimum flow rate             | 0.015 m <sup>3</sup> /h |
| Accuracy at minimum flow rate | 5%                      |

The design of flow-meters requires a thorough technical assessment of the system where the device will be used. The following is a list of areas to consider:

- Minimum and maximum flow rate at maximum allowable error in the system
- Transitional flow rate
- Instantaneous and total quantity pumped over time
- Accuracy of the meter within prescribed limits per applicable standards
- Pressure in the system
- Operating temperature range

The appropriate ultrasonic sensor and the proper electronics for interfacing to the sensor are determined based on the system requirements. The following is a list of specifications applicable to the sensor/assembly used in the system:

- Excitation frequency
- Excitation source voltage
- Pipe diameter
- Distance between the transducers (or reflectors)

## 9.2.2 Detailed Design Procedure

The following subsections describe the detailed design procedure for a flow meter application.

### 9.2.2.1 Flow Meter Regulations and Accuracy

If the flow meter is intended for residential applications, it must be designed to meet the required standards. For example, per the INTERNATIONAL ORGANIZATION OF LEGAL METROLOGY (OIML), the metrological requirements of water meters are defined by the values of Q1, Q2, Q3 and Q4, which are described in [Table 26](#).

**Table 26. Flow-rate Zones per OIML**

| FLOW-RATE ZONE | DESCRIPTION  |
|----------------|--|
| Q1             | Lowest flow rate at which the meter is to operate within the maximum permissible errors.   |
| Q2             | Flow rate between the permanent flow rate and the minimum flow rate that divides the flow rate range into two zones, the upper flow rate zone and the lower flow rate zone, each characterized by its own maximum permissible errors.        |
| Q3             | Highest flow rate within the rated operating condition at which the meter is to operate within the maximum permissible errors.   |
| Q4             | Highest flow rate at which the meter is to operate for a short period of time within the maximum permissible errors, while maintaining its metrological performance when it is subsequently operating within the rated operating conditions. |

A water meter is designated by the numerical value of Q3 in m<sup>3</sup>/h and the ratio Q3/Q1. The value of Q3 and the ratio of Q3/Q1 are selected from the lists provided in the OIML standards.

Water meters have to be designed and manufactured such that their errors do not exceed the maximum permissible errors (MPE) defined in the standards. For example, in OIML standards, water meters need to be designated as either accuracy class 1 or accuracy class 2, according to the requirements.

For class 1 water meters, the maximum permissible error in the upper flow rate zone ( $Q2 \leq Q \leq Q4$ ) is  $\pm 1\%$ , for temperatures from 0.1°C to 30°C, and  $\pm 2\%$  for temperatures greater than 30°C. The maximum permissible error for the lower flow-rate zone ( $Q1 \leq Q < Q2$ ) is  $\pm 3\%$ , regardless of the temperature range.

For class 2 water meters, the maximum permissible error for the upper flow rate zone ( $Q2 \leq Q \leq Q4$ ) is  $\pm 2\%$ , for temperatures from 0.1°C to 30°C, and  $\pm 3\%$  for temperatures greater than 30°C. The maximum permissible error for the lower flow rate zone ( $Q1 \leq Q < Q2$ ) is  $\pm 5\%$  regardless of the temperature range.

The flow meter accuracy specified in the standards dictates the required accuracy in the electronics used for driving the ultrasonic transducers, circuits in the receiver path, and time measurement sub circuits. The stringent accuracy required at lower flow rates would require a very low noise signal chain in the transmitter and receiver circuits used in ultrasonic flow meters, as well as the ability to measure picosecond time intervals.

### 9.2.2.2 Transmit Time in Ultrasonic Flow Meters

Transit-time ultrasonic flow meters works based on the principle that sound waves in a moving fluid travel faster in the direction of flow (downstream), and slower in the opposite direction of flow (upstream).

The system requires at least two transducers. The first transducer operates as a transmitter during the upstream cycle and as a receiver during the downstream cycle, and the second transducer operates as a receiver during the upstream cycle and as a transmitter during the downstream cycle. An ultrasonic flow meter operates by alternating transmit and receive cycles between the pair of transducers and accurately measuring the time-of-flight both directions.

In this example, the upstream TOF is defined as:

$$t_{BA} = \frac{l}{(c - v)}$$

where

- $l$  is the path length between the two transducers in meters (m)
  - $c$  is the speed of sound in water in meters per second (m/s)
  - $v$  is the velocity of the water in the pipe in meters per second (m/s)
- (4)

In this example, the downstream TOF is defined as:

$$t_{AB} = \frac{l}{(c + v)}$$

where

- $l$  is the path length between the two transducers in meters (m)
  - $c$  is the speed of sound in water in meters per second (m/s)
  - $v$  is the velocity of the water in the pipe in meters per second (m/s)
- (5)

The difference of TOF is defined as:

$$\Delta TOF = t_{BA} - t_{AB}$$

where

- $t_{BA}$  is the upstream TOF from transducer B to transducer A in seconds (s)
  - $t_{AB}$  is the downstream TOF from transducer A to transducer B in seconds (s)
- (6)

After the difference in time-of-flight ( $\Delta TOF$ ) is calculated, the water velocity inside the pipe can be related to the  $\Delta TOF$  using the following equation:

$$v = \frac{\Delta TOF \times c^2}{2 \times l}$$

where

- $c$  is the speed of sound in water in meters per second (m/s)
  - $l$  is the path length between the two transducers in meters (m)
- (7)

Finally, the mass flow rate can be calculated as follows:

$$Q = k \times v \times A$$

where

- $k$  is the flow-meter constant
  - $v$  is the velocity of the water in the pipe in meters per second (m/s)
  - $A$  is the cross-section area of the pipe in meters-squared (m<sup>2</sup>)
- (8)

### 9.2.2.3 $\Delta TOF$ Accuracy Requirement Calculation

Based on the minimum mass flow requirement and accuracy requirements in [Table 25](#), the  $\Delta TOF$  accuracy needed can be calculated as follows:

1. Convert the mass flow rate to m<sup>3</sup>/s:

$$Q = (0.015 \text{ m}^3/\text{h}) \left( \frac{1 \text{ h}}{3600 \text{ s}} \right) = 4.167 \times 10^{-6} \text{ m}^3/\text{s}$$

2. Calculate the flow velocity assuming  $k = 1$ :

$$v = \frac{Q}{kA} = \frac{4.167 \times 10^{-6} \text{ m}^3/\text{s}}{\pi \left( \frac{0.015 \text{ m}}{2} \right)^2} = 0.0236 \text{ m/s}$$

3. Calculate the  $\Delta\text{TOF}$  for the given speed of sound. In this example, a speed of sound  $c = 1400 \text{ m/s}$  is assumed:

$$\Delta\text{TOF} = \frac{2 \times l \times v}{c^2} = \frac{(2)(0.06 \text{ m})(0.0236 \text{ m/s})}{1400 \text{ m/s}^2} = 1.445 \text{ ns}$$

4. The requirement of 5% accuracy for minimum flow will result in a  $\Delta\text{TOF}$  accuracy of:

$$\Delta\text{TOF}_{\text{error}} = (0.05)(1.445 \text{ ns}) = 72.25 \text{ ps}$$

For this reason, this system requires a high accuracy timer/stopwatch that can measure the lower flow rate state.


The TDC1000 ultrasonic analog-front-end is used to drive the transmitter, amplify and filter the received signal and conditioning the echo for START and STOP pulse generation. The TDC7200 ps-accurate timer is used to measure the time interval between the rising edge of the START pulse and the rising edge of the STOP pulse produced by the TDC1000.

The microcontroller should first configure the TDC7200 and the TDC1000 for the measurement. When the microcontroller issues a start command to the TDC7200 via the SPI interface, the TDC7200 sends a trigger pulse to the TRIGGER pin of the TDC1000. When the TDC1000 drives the transmit transducer, a synchronous START pulse is produced on the START pin, which commands the TDC7200 to start its counters. When a valid echo pulse is received on the receive transducer, the TDC1000 generates a STOP pulse on the STOP pin, which commands the TDC7200 to stop its counters. This procedure is repeated for the upstream and downstream cycles.

A temperature measurement can be performed and the result can be used to correct for temperature dependency of the speed of sound.

### 9.2.3 Application Curves

Figure 46 , Figure 47, and Figure 48 show data and histograms created with data collected under a zero flow condition at room temperature. A simple offset calibration has been applied, where the overall average of the data is subtracted from the data.

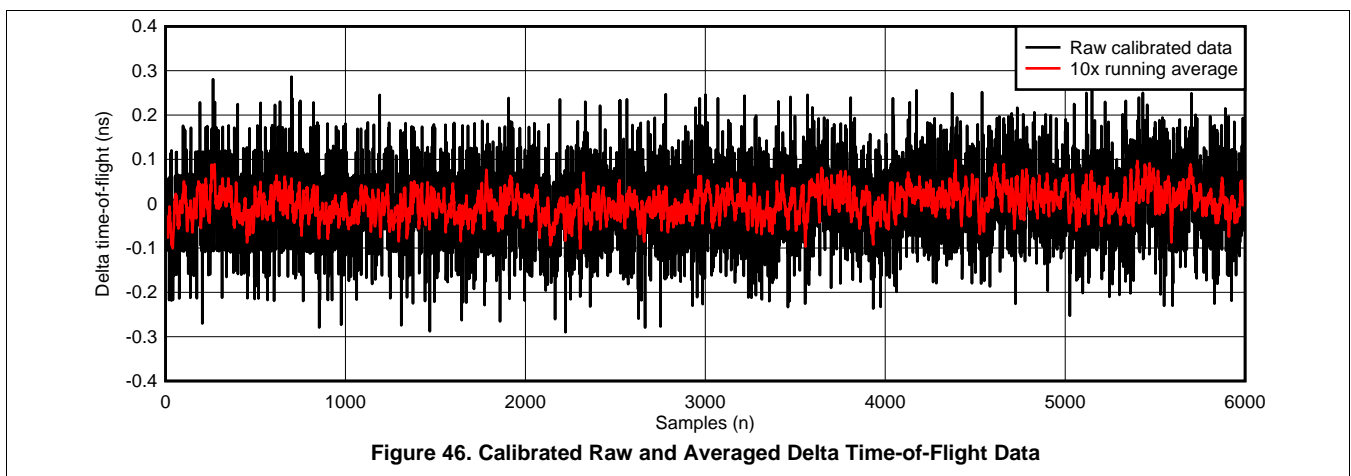

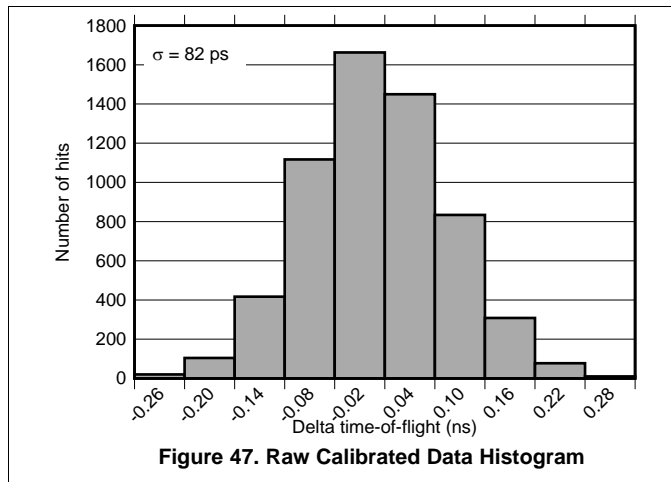


Figure 47. Raw Calibrated Data Histogram

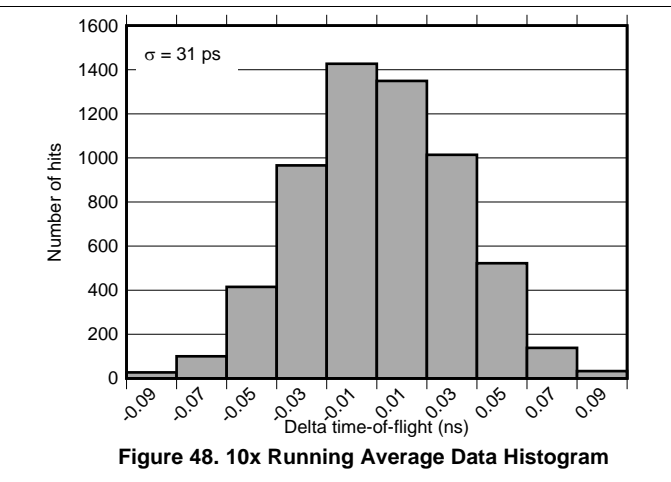


Figure 48. 10x Running Average Data Histogram

### 9.3 Post Filtering Recommendations

For application such as flow meters where conversion results are accumulated over a long period of time, post filtering is not required. However, for applications where a specific action is taken based on individual conversion results, post filtering is recommended. One advantage of post filtering is to remove the conversion results that are outside of the normal distribution.

One such post filtering method commonly applied by an MCU is the Median Filter Method. The median of a finite number of conversion results can be found by arranging all the conversions from the lowest value to the highest value, and picking the middle one. For example, a conversion result of {50, 51, 49, 40, 51} can be rearranged from lowest to highest {40, 49, 50, 51, 51}, and the median value after applying the Median Filter Method is 50.

### 9.4 CLOCK Recommendations

A stable, known reference clock is crucial to the ability to measure time, regardless of the time measuring device. Two parameters of a clock source primarily affect the ability to measure time: accuracy and jitter. The following subsections will discuss recommendations for the CLOCK in order to increase accuracy and reduce jitter.

#### 9.4.1 CLOCK Accuracy

CLOCK sources are typically specified with an accuracy value as the clock period is not exactly equal to the nominal value specified. For example, an 8 MHz clock reference may have a 20 ppm accuracy. The true value of the clock period therefore has an error of  $\pm 20\text{ppm}$ , and the real frequency is in the range 7.99984 MHz to 8.00016 MHz [ $8\text{ MHz} \pm (8\text{ MHz}) \times (20/10^6)$ ].

If the clock accuracy is at this boundary, but the reference time used to calculate the time of flight relates to the nominal 8 MHz clock period, then the time measured will be affected by this error. For example, if the time period measured is 50  $\mu\text{s}$ , and the 8MHz reference clock has +50ppm of error in frequency, but the time measured refers to the 125 ns period (1/8 MHz), then the 50  $\mu\text{s}$  time period will have an error of  $50\mu\text{s} \times 50/1000000 = 2.5\text{ ns}$ .

In summary, a clock inaccuracy translates proportionally to a time measurement error.

#### 9.4.2 CLOCK Jitter

Clock jitter introduces uncertainty into a time measurement, rather than inaccuracy. As shown in Figure 49, the jitter accumulates on each clock cycle so the uncertainty associated to a time measurement is a function of the clock jitter and the number of clock cycles measured.

Clock\_Jitter\_Uncertainty =  $(\sqrt{n}) \times (\theta_{\text{JITTER}})$ , where n is the number of clock cycles counted, and  $\theta_{\text{JITTER}}$  is the cycle-to-cycle jitter of the clock.

For example, if the time measured is 50  $\mu\text{s}$  using an 8 MHz reference clock,  $n = 50\text{ }\mu\text{s} / (1/8\text{ MHz}) = 400$  clock cycles. If the RMS cycle-to-cycle jitter,  $\theta_{\text{JITTER}} = 10\text{ ps}$ , then the RMS uncertainty introduced in a single measurement is in the order of  $(\sqrt{n}) \times (\theta_{\text{JITTER}}) = 200\text{ ps}$ .

### CLOCK Recommendations (continued)

Because the effect of jitter is random, averaging or accumulating time results reduces the effect of the uncertainty introduced. If the time is measured  $m$  times and the result is averaged, then the uncertainty is reduced to:  $\text{Clock\_Jitter\_Uncertainty} = (\theta_{\text{JITTER}}) / (\sqrt{m})$ .

For example, if 64 averages are performed in the example above, then the jitter-related uncertainty is reduced to 25 ps RMS.

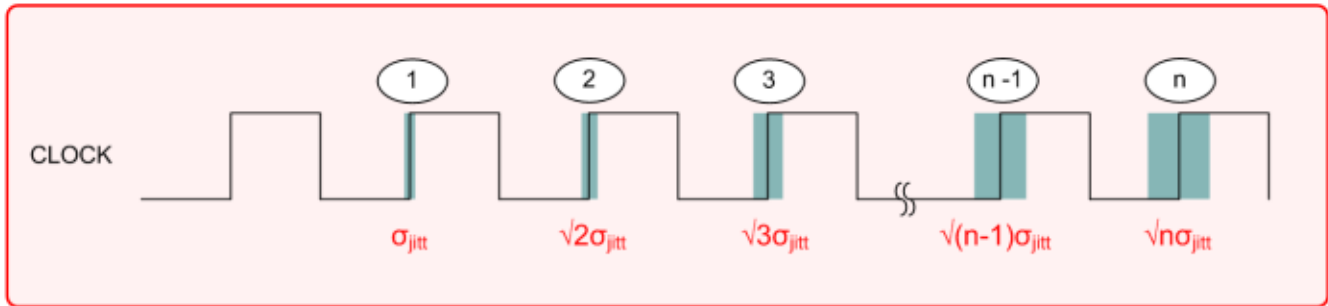


Figure 49. CLOCK Jitter

## 10 Power Supply Recommendations

The analog circuitry of the TDC7200 is designed to operate from an input voltage supply range between 2 V and 3.6 V. It is recommended to place a 100 nF ceramic bypass capacitor to ground as close as possible to the VDD pins. In addition, an electrolytic or tantalum capacitor with value greater than 1  $\mu$ F is recommended. The bulk capacitor does not need to be in close vicinity with the TDC7200 and could be close to the voltage source terminals or at the output of the voltage regulators powering the TDC7200.

## 11 Layout

### 11.1 Layout Guidelines

- In a 4-layer board design, the recommended layer stack order from top to bottom is: signal, ground, power and signal.
- Bypass capacitors should be placed in close proximity to the VDD pin.
- The length of the START and STOP traces from the TDC7200 to the stopwatch/MCU should be matched to prevent uneven signal delays. Also, avoid unnecessary via-holes on these traces and keep the routing as short/direct as possible to minimize parasitic capacitance on the PCB.
- Route the SPI signal traces close together. Place a series resistor at the source of DOUT (close to the TDC7200) and series resistors at the sources of DIN, SCLK, and CSB (close to the master MCU).

11.2 Layout Example

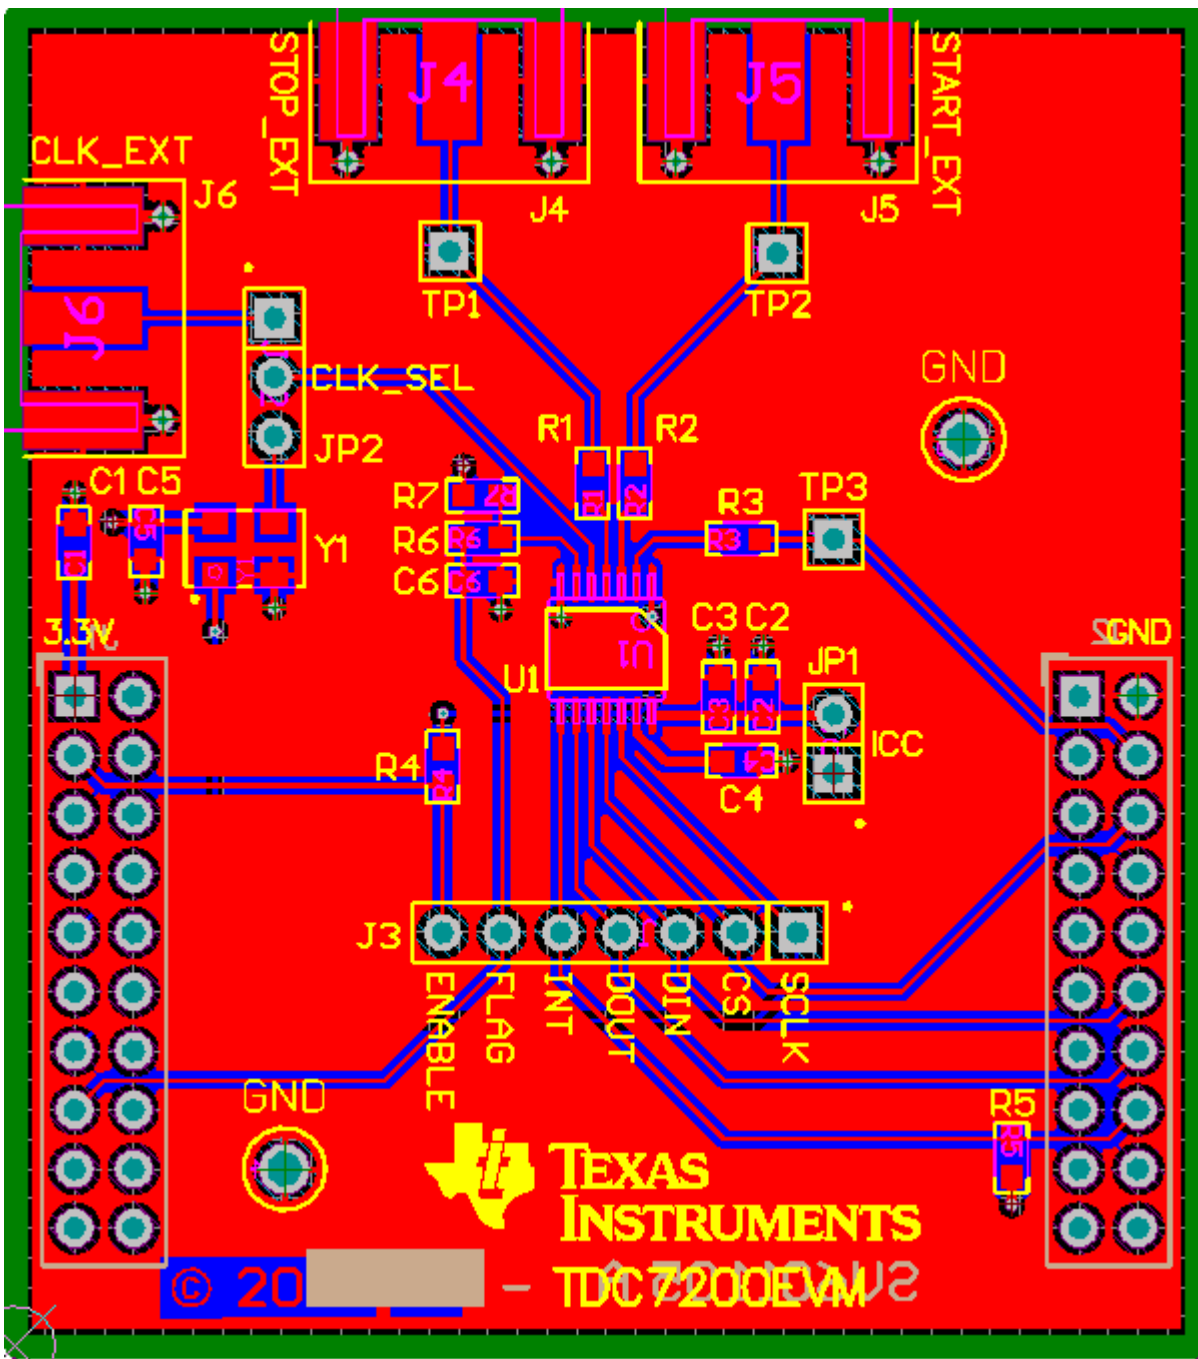


Figure 50. TDC7200EVM Layout

## 12 Device and Documentation Support

### 12.1 Documentation Support

#### 12.1.1 Related Documentation

For related documentation see the following:

- TDC1000 : Ultrasonic Sensing Analog Front End for Level, Concentration, Flow & Proximity Sensing Applications.

### 12.2 Trademarks

SPI is a trademark of Motorola.

All other trademarks are the property of their respective owners.

### 12.3 Electrostatic Discharge Caution



These devices have limited built-in ESD protection. The leads should be shorted together or the device placed in conductive foam during storage or handling to prevent electrostatic damage to the MOS gates.

### 12.4 Glossary

[SLYZ022](#) — *TI Glossary*.

This glossary lists and explains terms, acronyms, and definitions.

## 13 Mechanical, Packaging, and Orderable Information

The following pages include mechanical, packaging, and orderable information. This information is the most current data available for the designated devices. This data is subject to change without notice and revision of this document. For browser-based versions of this data sheet, refer to the left-hand navigation.

**PACKAGING INFORMATION**

| Orderable Device | Status<br>(1) | Package Type | Package Drawing | Pins | Package Qty | Eco Plan<br>(2)         | Lead/Ball Finish<br>(6) | MSL Peak Temp<br>(3) | Op Temp (°C) | Device Marking<br>(4/5) | Samples |
|------------------|---------------|--------------|-----------------|------|-------------|-------------------------|-------------------------|----------------------|--------------|-------------------------|---------|
| TDC7200PW        | PREVIEW       | TSSOP        | PW              | 14   | 90          | Green (RoHS & no Sb/Br) | CU NIPDAU               | Level-1-260C-UNLIM   | -40 to 85    | T7200                   |         |
| TDC7200PWR       | PREVIEW       | TSSOP        | PW              | 14   | 2000        | Green (RoHS & no Sb/Br) | CU NIPDAU               | Level-1-260C-UNLIM   | -40 to 85    | T7200                   |         |

(1) The marketing status values are defined as follows:

**ACTIVE:** Product device recommended for new designs.

**LIFEBUY:** TI has announced that the device will be discontinued, and a lifetime-buy period is in effect.

**NRND:** Not recommended for new designs. Device is in production to support existing customers, but TI does not recommend using this part in a new design.

**PREVIEW:** Device has been announced but is not in production. Samples may or may not be available.

**OBsolete:** TI has discontinued the production of the device.

(2) Eco Plan - The planned eco-friendly classification: Pb-Free (RoHS), Pb-Free (RoHS Exempt), or Green (RoHS & no Sb/Br) - please check <http://www.ti.com/productcontent> for the latest availability information and additional product content details.

**TBD:** The Pb-Free/Green conversion plan has not been defined.

**Pb-Free (RoHS):** TI's terms "Lead-Free" or "Pb-Free" mean semiconductor products that are compatible with the current RoHS requirements for all 6 substances, including the requirement that lead not exceed 0.1% by weight in homogeneous materials. Where designed to be soldered at high temperatures, TI Pb-Free products are suitable for use in specified lead-free processes.

**Pb-Free (RoHS Exempt):** This component has a RoHS exemption for either 1) lead-based flip-chip solder bumps used between the die and package, or 2) lead-based die adhesive used between the die and leadframe. The component is otherwise considered Pb-Free (RoHS compatible) as defined above.

**Green (RoHS & no Sb/Br):** TI defines "Green" to mean Pb-Free (RoHS compatible), and free of Bromine (Br) and Antimony (Sb) based flame retardants (Br or Sb do not exceed 0.1% by weight in homogeneous material)

(3) MSL, Peak Temp. - The Moisture Sensitivity Level rating according to the JEDEC industry standard classifications, and peak solder temperature.

(4) There may be additional marking, which relates to the logo, the lot trace code information, or the environmental category on the device.

(5) Multiple Device Markings will be inside parentheses. Only one Device Marking contained in parentheses and separated by a "~" will appear on a device. If a line is indented then it is a continuation of the previous line and the two combined represent the entire Device Marking for that device.


(6) Lead/Ball Finish - Orderable Devices may have multiple material finish options. Finish options are separated by a vertical ruled line. Lead/Ball Finish values may wrap to two lines if the finish value exceeds the maximum column width.

**Important Information and Disclaimer:** The information provided on this page represents TI's knowledge and belief as of the date that it is provided. TI bases its knowledge and belief on information provided by third parties, and makes no representation or warranty as to the accuracy of such information. Efforts are underway to better integrate information from third parties. TI has taken and continues to take reasonable steps to provide representative and accurate information but may not have conducted destructive testing or chemical analysis on incoming materials and chemicals. TI and TI suppliers consider certain information to be proprietary, and thus CAS numbers and other limited information may not be available for release.

In no event shall TI's liability arising out of such information exceed the total purchase price of the TI part(s) at issue in this document sold by TI to Customer on an annual basis.

PW (R-PDSO-G14)

PLASTIC SMALL OUTLINE

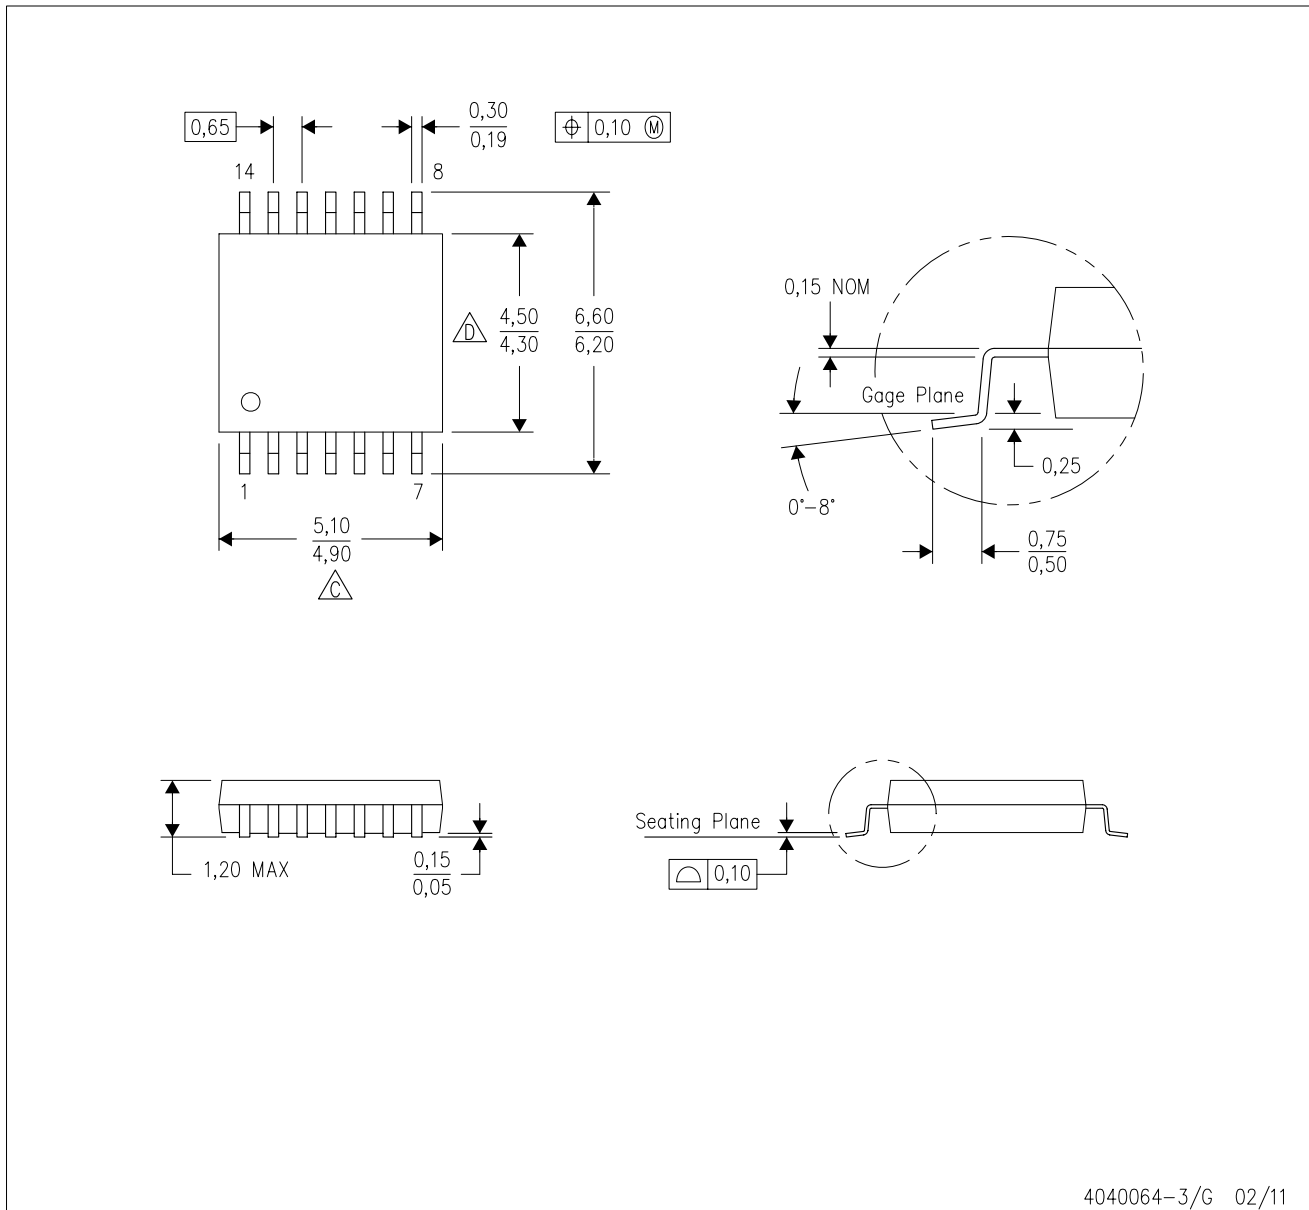

4040064-3/G 02/11

- NOTES:
- A. All linear dimensions are in millimeters. Dimensioning and tolerancing per ASME Y14.5M-1994.
  - B. This drawing is subject to change without notice.
  - C. Body length does not include mold flash, protrusions, or gate burrs. Mold flash, protrusions, or gate burrs shall not exceed 0,15 each side.
  - D. Body width does not include interlead flash. Interlead flash shall not exceed 0,25 each side.
  - E. Falls within JEDEC MO-153

## IMPORTANT NOTICE

Texas Instruments Incorporated and its subsidiaries (TI) reserve the right to make corrections, enhancements, improvements and other changes to its semiconductor products and services per JESD46, latest issue, and to discontinue any product or service per JESD48, latest issue. Buyers should obtain the latest relevant information before placing orders and should verify that such information is current and complete. All semiconductor products (also referred to herein as "components") are sold subject to TI's terms and conditions of sale supplied at the time of order acknowledgment.

TI warrants performance of its components to the specifications applicable at the time of sale, in accordance with the warranty in TI's terms and conditions of sale of semiconductor products. Testing and other quality control techniques are used to the extent TI deems necessary to support this warranty. Except where mandated by applicable law, testing of all parameters of each component is not necessarily performed.

TI assumes no liability for applications assistance or the design of Buyers' products. Buyers are responsible for their products and applications using TI components. To minimize the risks associated with Buyers' products and applications, Buyers should provide adequate design and operating safeguards.

TI does not warrant or represent that any license, either express or implied, is granted under any patent right, copyright, mask work right, or other intellectual property right relating to any combination, machine, or process in which TI components or services are used. Information published by TI regarding third-party products or services does not constitute a license to use such products or services or a warranty or endorsement thereof. Use of such information may require a license from a third party under the patents or other intellectual property of the third party, or a license from TI under the patents or other intellectual property of TI.

Reproduction of significant portions of TI information in TI data books or data sheets is permissible only if reproduction is without alteration and is accompanied by all associated warranties, conditions, limitations, and notices. TI is not responsible or liable for such altered documentation. Information of third parties may be subject to additional restrictions.

Resale of TI components or services with statements different from or beyond the parameters stated by TI for that component or service voids all express and any implied warranties for the associated TI component or service and is an unfair and deceptive business practice. TI is not responsible or liable for any such statements.

Buyer acknowledges and agrees that it is solely responsible for compliance with all legal, regulatory and safety-related requirements concerning its products, and any use of TI components in its applications, notwithstanding any applications-related information or support that may be provided by TI. Buyer represents and agrees that it has all the necessary expertise to create and implement safeguards which anticipate dangerous consequences of failures, monitor failures and their consequences, lessen the likelihood of failures that might cause harm and take appropriate remedial actions. Buyer will fully indemnify TI and its representatives against any damages arising out of the use of any TI components in safety-critical applications.

In some cases, TI components may be promoted specifically to facilitate safety-related applications. With such components, TI's goal is to help enable customers to design and create their own end-product solutions that meet applicable functional safety standards and requirements. Nonetheless, such components are subject to these terms.

No TI components are authorized for use in FDA Class III (or similar life-critical medical equipment) unless authorized officers of the parties have executed a special agreement specifically governing such use.

Only those TI components which TI has specifically designated as military grade or "enhanced plastic" are designed and intended for use in military/aerospace applications or environments. Buyer acknowledges and agrees that any military or aerospace use of TI components which have **not** been so designated is solely at the Buyer's risk, and that Buyer is solely responsible for compliance with all legal and regulatory requirements in connection with such use.

TI has specifically designated certain components as meeting ISO/TS16949 requirements, mainly for automotive use. In any case of use of non-designated products, TI will not be responsible for any failure to meet ISO/TS16949.

### Products

|                              |  |
|------------------------------|--|
| Audio                        | <a href="http://www.ti.com/audio">www.ti.com/audio</a>                               |
| Amplifiers                   | <a href="http://amplifier.ti.com">amplifier.ti.com</a>                               |
| Data Converters              | <a href="http://dataconverter.ti.com">dataconverter.ti.com</a>                       |
| DLP® Products                | <a href="http://www.dlp.com">www.dlp.com</a>   |
| DSP                          | <a href="http://dsp.ti.com">dsp.ti.com</a>   |
| Clocks and Timers            | <a href="http://www.ti.com/clocks">www.ti.com/clocks</a>                             |
| Interface                    | <a href="http://interface.ti.com">interface.ti.com</a>                               |
| Logic                        | <a href="http://logic.ti.com">logic.ti.com</a>                                       |
| Power Mgmt                   | <a href="http://power.ti.com">power.ti.com</a>                                       |
| Microcontrollers             | <a href="http://microcontroller.ti.com">microcontroller.ti.com</a>                   |
| RFID                         | <a href="http://www.ti-rfid.com">www.ti-rfid.com</a>                                 |
| OMAP Applications Processors | <a href="http://www.ti.com/omap">www.ti.com/omap</a>                                 |
| Wireless Connectivity        | <a href="http://www.ti.com/wirelessconnectivity">www.ti.com/wirelessconnectivity</a> |

### Applications

|                               |  |
|-------------------------------|--|
| Automotive and Transportation | <a href="http://www.ti.com/automotive">www.ti.com/automotive</a>                         |
| Communications and Telecom    | <a href="http://www.ti.com/communications">www.ti.com/communications</a>                 |
| Computers and Peripherals     | <a href="http://www.ti.com/computers">www.ti.com/computers</a>                           |
| Consumer Electronics          | <a href="http://www.ti.com/consumer-apps">www.ti.com/consumer-apps</a>                   |
| Energy and Lighting           | <a href="http://www.ti.com/energy">www.ti.com/energy</a>                                 |
| Industrial                    | <a href="http://www.ti.com/industrial">www.ti.com/industrial</a>                         |
| Medical                       | <a href="http://www.ti.com/medical">www.ti.com/medical</a>                               |
| Security                      | <a href="http://www.ti.com/security">www.ti.com/security</a>                             |
| Space, Avionics and Defense   | <a href="http://www.ti.com/space-avionics-defense">www.ti.com/space-avionics-defense</a> |
| Video and Imaging             | <a href="http://www.ti.com/video">www.ti.com/video</a>                                   |

### TI E2E Community

[e2e.ti.com](http://e2e.ti.com)